


Sample Name: Ketotifen Fumarate STD 20 ppm

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Acq. Instrument : hplc -2                    Location  : Vial 1
Injection Date  : 12/3/2024 9:46:32 AM        Inj       :    3
                                           Inj Volume: 20.000 µl

Acq. Method     : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M
Last changed    : 12/3/2024 9:28:59 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M (Sequence Method)
Last changed    : 12/4/2024 5:33:29 PM by SYSTEM
                  (modified after loading)
Additional Info : Peak(s) manually integrated
=====
```

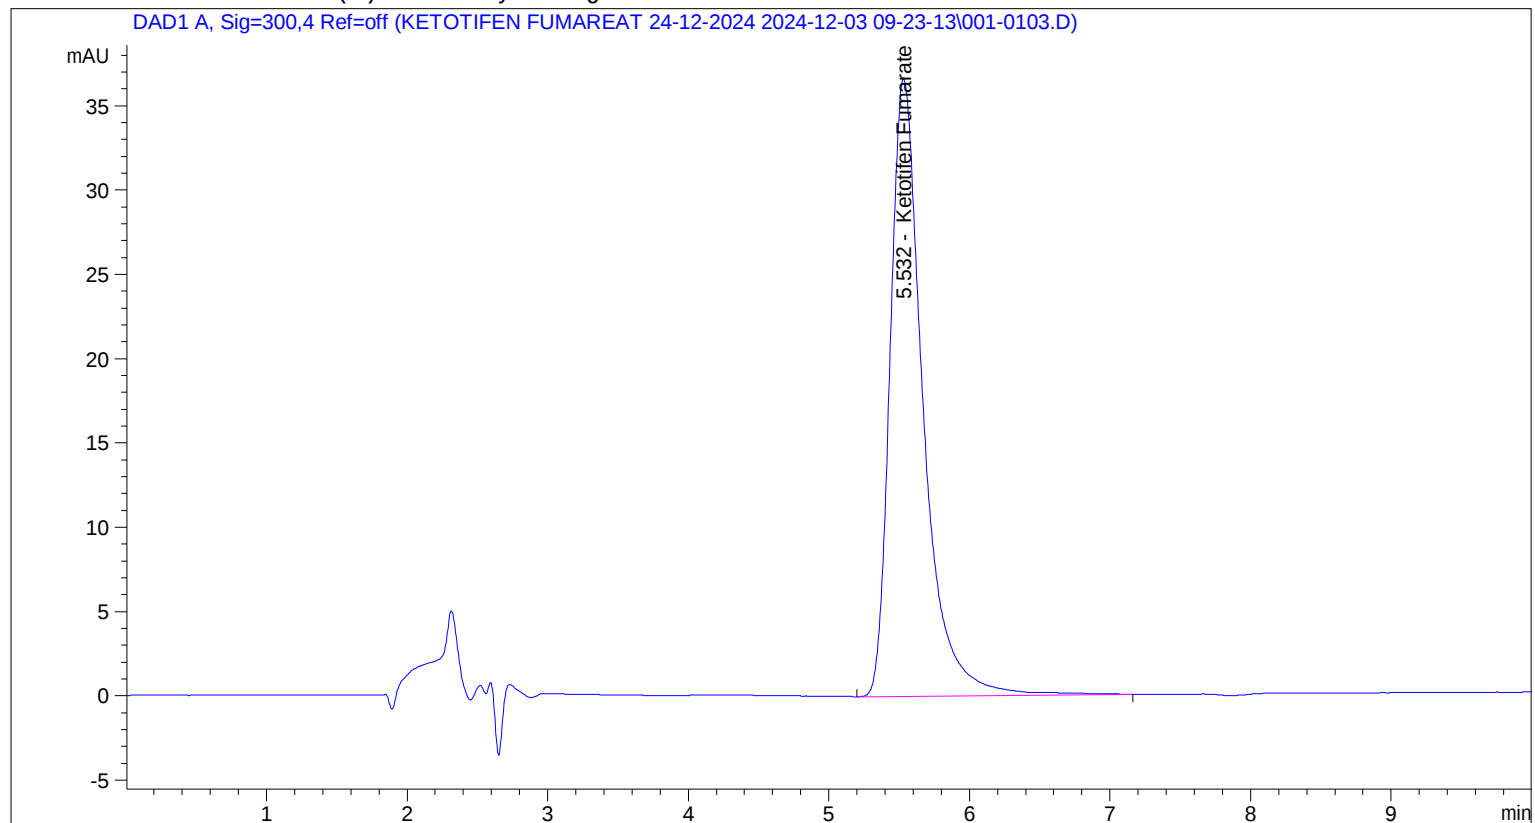

```
=====
                        Area Percent Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified : 12/4/2024 5:33:29 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=300,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	5.532	BB	0.2463	597.43060	100.0000	Ketotifen Fumarate

Totals : 597.43060

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Invalid calibration curve, (Ketotifen Fumarate)

=====

*** End of Report ***