


Sample Name: 2.5 ppm

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Acq. Instrument : hplc -2                    Location  : Vial 4
Injection Date  : 12/3/2024 11:03:50 AM      Inj       :    1
                                           Inj Volume: 20.000 µl

Acq. Method     : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M
Last changed    : 12/3/2024 10:33:10 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M (Sequence Method)
Last changed    : 12/4/2024 5:33:29 PM by SYSTEM
                  (modified after loading)

Additional Info : Peak(s) manually integrated
  
```

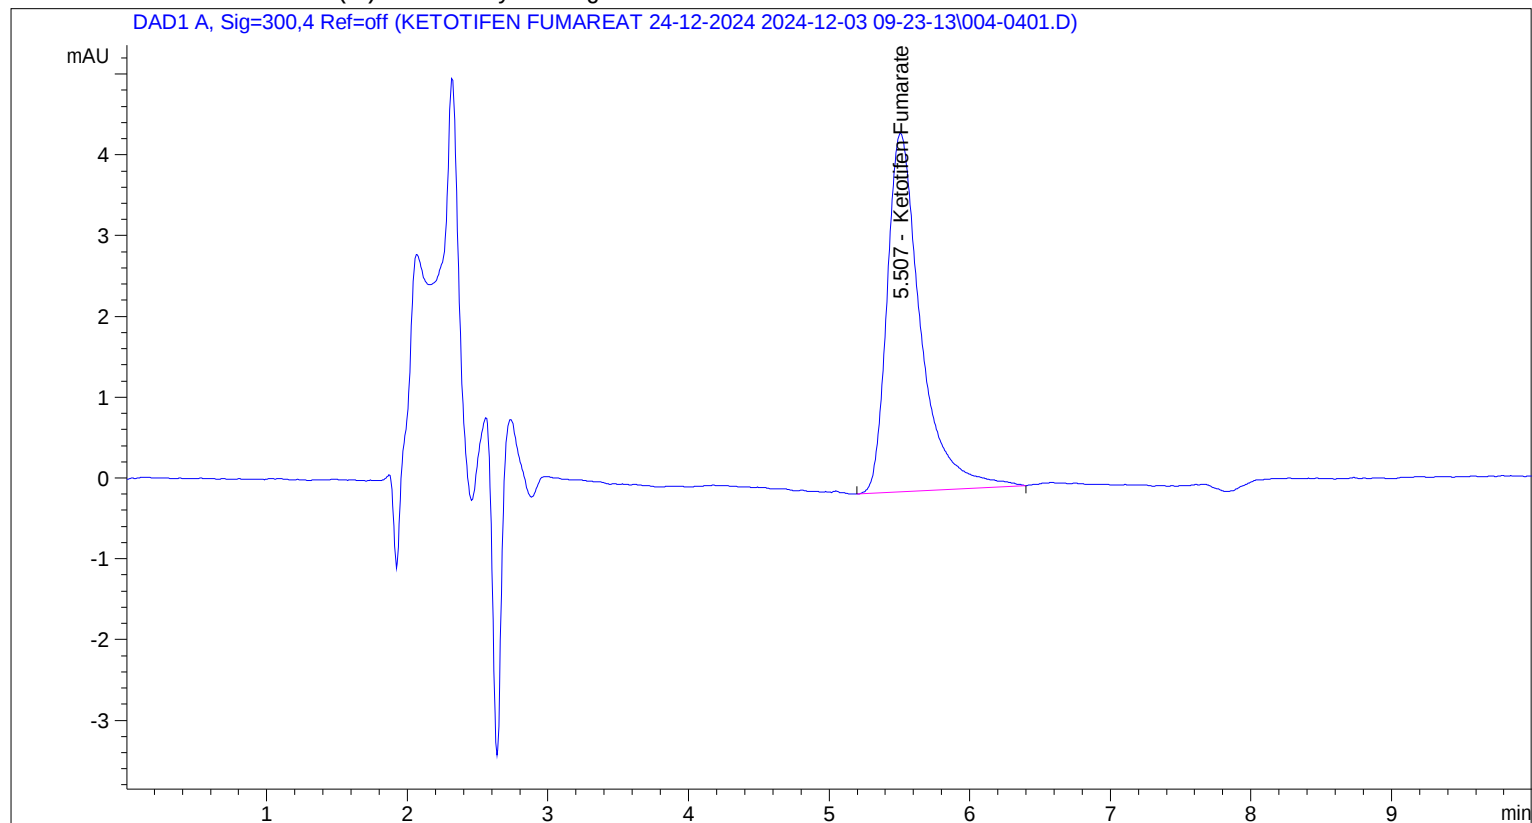

```

=====
                        Area Percent Report
=====
  
```

```

Sorted By      :      Signal
Calib. Data Modified :      12/4/2024 5:33:29 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=300,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	5.507	BB	0.2471	73.55404	100.0000	Ketotifen Fumarate

Totals : 73.55404

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Invalid calibration curve, (Ketotifen Fumarate)

=====

*** End of Report ***