


Sample Name: 2.5 ppm

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Acq. Instrument : hplc -2                    Location  : Vial 4
Injection Date  : 12/3/2024 11:14:53 AM      Inj       :    2
                                           Inj Volume: 20.000 µl

Acq. Method     : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M
Last changed    : 12/3/2024 10:33:10 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M (Sequence Method)
Last changed    : 12/4/2024 5:33:29 PM by SYSTEM
                  (modified after loading)
Additional Info : Peak(s) manually integrated
=====
```

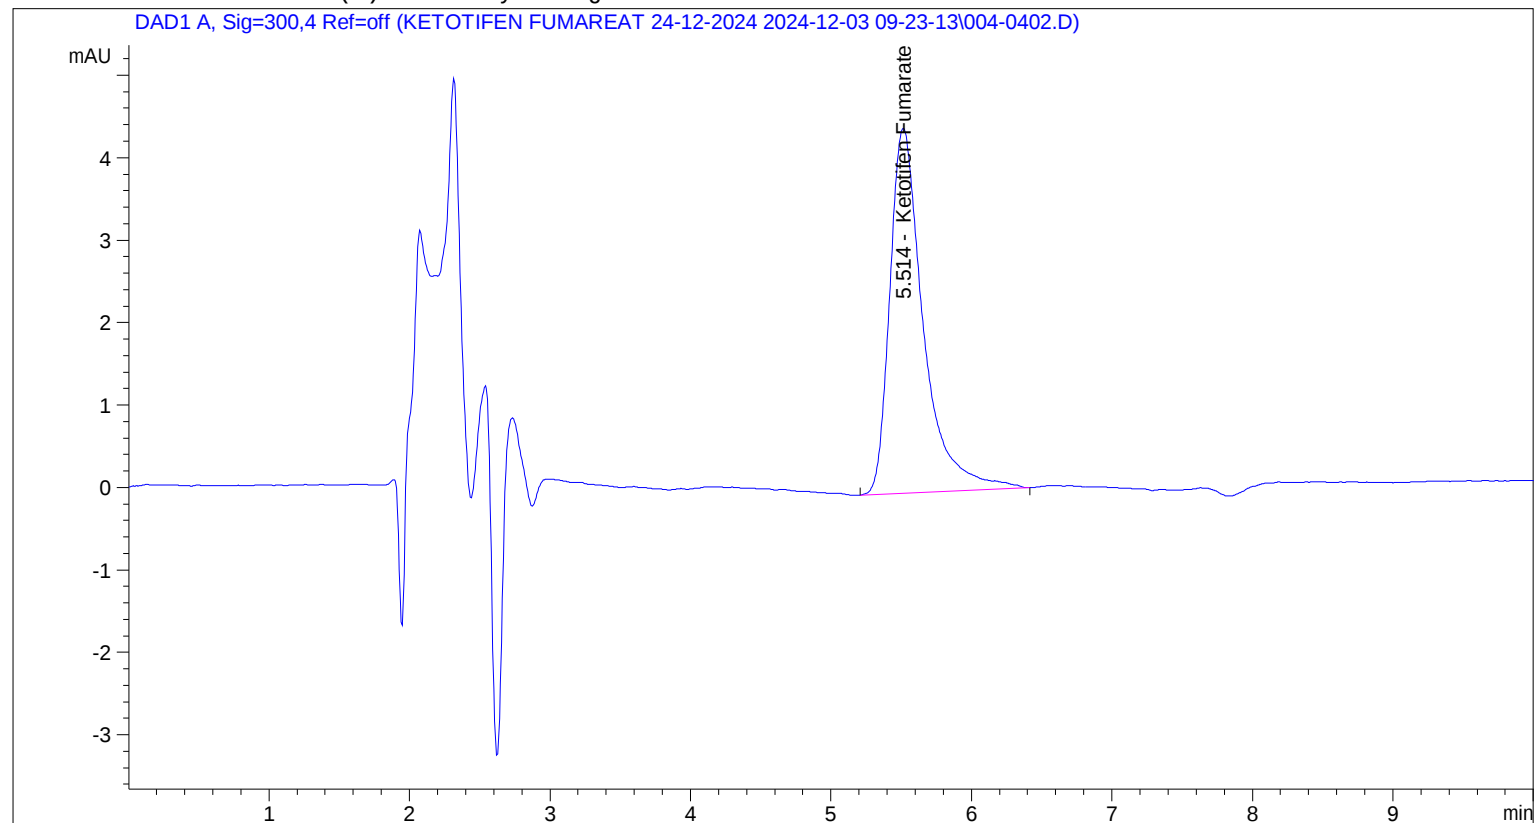

```
=====
                        Area Percent Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified : 12/4/2024 5:33:29 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=300,4 Ref=off

| Peak # | RetTime [min] | Type | Width [min] | Area [mAU*s] | Area %   | Name               |
|--------|---------------|------|-------------|--------------|----------|--------------------|
| 1      | 5.514         | BB   | 0.2481      | 73.64650     | 100.0000 | Ketotifen Fumarate |

Totals : 73.64650

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Invalid calibration curve, (Ketotifen Fumarate)

=====

\*\*\* End of Report \*\*\*