


Sample Name: Ketotifen fumarate STD 40ppm

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : hplc -2                      Location : Vial 1
Injection Date  : 12/3/2024 6:27:40 AM
                                           Inj Volume : 20.000 µl

Acq. Method     : C:\CHEM32\1\METHODS\KETOTIFEN FUMARATE.M
Last changed    : 12/3/2024 5:40:25 AM by SYSTEM
                  (modified after loading)
Analysis Method : C:\CHEM32\1\METHODS\POTASSIUM SORBATE.M
Last changed    : 12/3/2024 10:18:10 AM by SYSTEM
                  (modified after loading)
Additional Info : Peak(s) manually integrated
=====
```

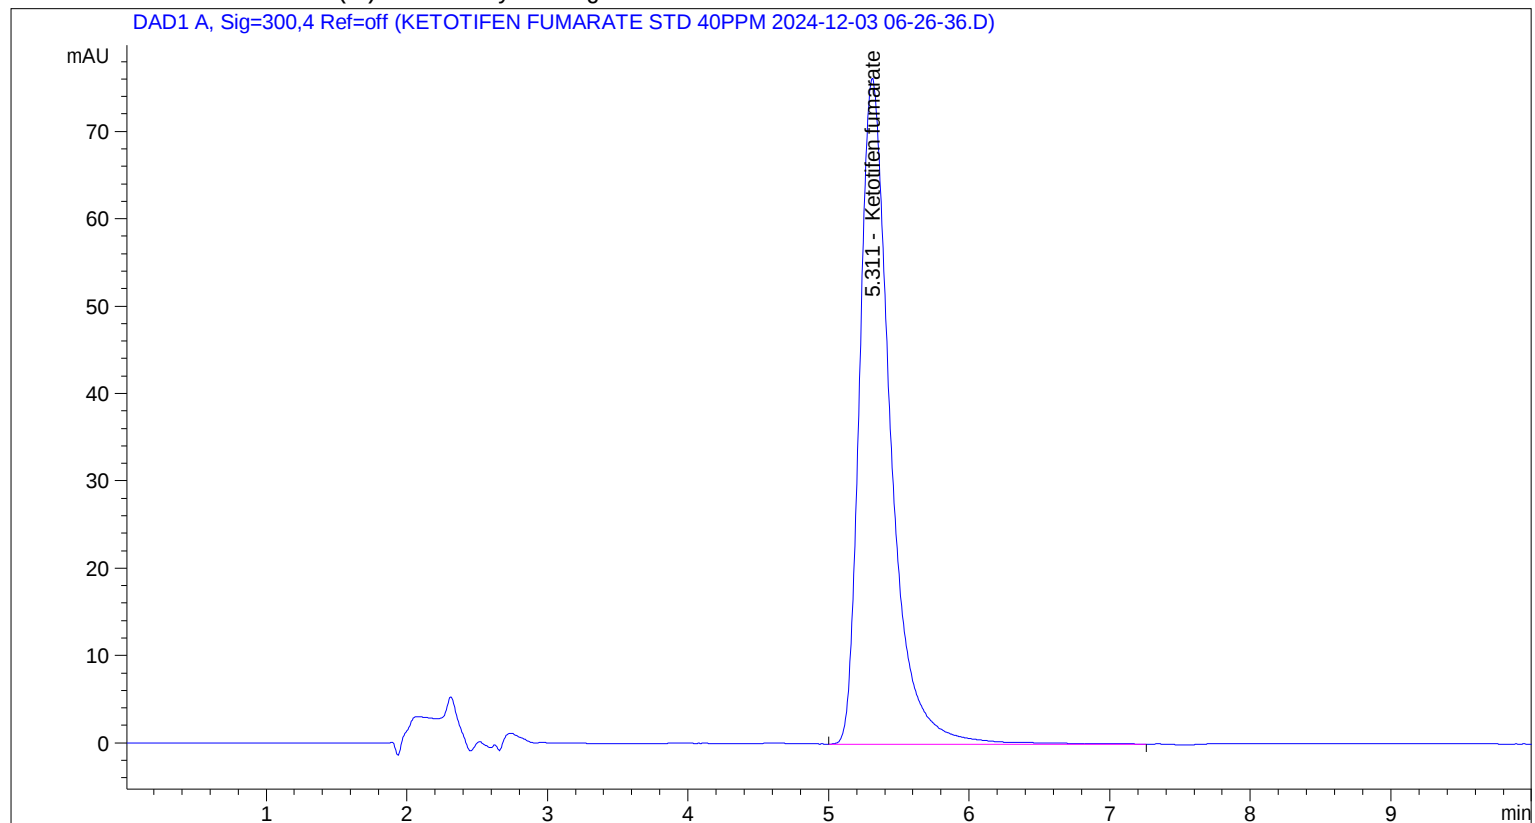

```
=====
                        Area Percent Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      12/3/2024 10:18:10 AM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=300,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	5.311	BB	0.2291	1156.82507	100.0000	Ketotifen fumarate

Totals : 1156.82507

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Invalid calibration curve, (Ketotifen fumarate)

=====

*** End of Report ***