


Sample Name: 5 ppm

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    3
Acq. Instrument : hplc -2                    Location  : Vial 3
Injection Date  : 12/3/2024 10:30:40 AM      Inj       :    1
                                           Inj Volume: 20.000 µl

Acq. Method     : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M
Last changed    : 12/3/2024 9:28:59 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\KETOTIFEN FUMAREAT 24-12-2024 2024-12-03 09-23-13
                  \KETOTIFEN FUMARATE.M (Sequence Method)
Last changed    : 12/4/2024 5:33:29 PM by SYSTEM
                  (modified after loading)
Additional Info : Peak(s) manually integrated
  
```

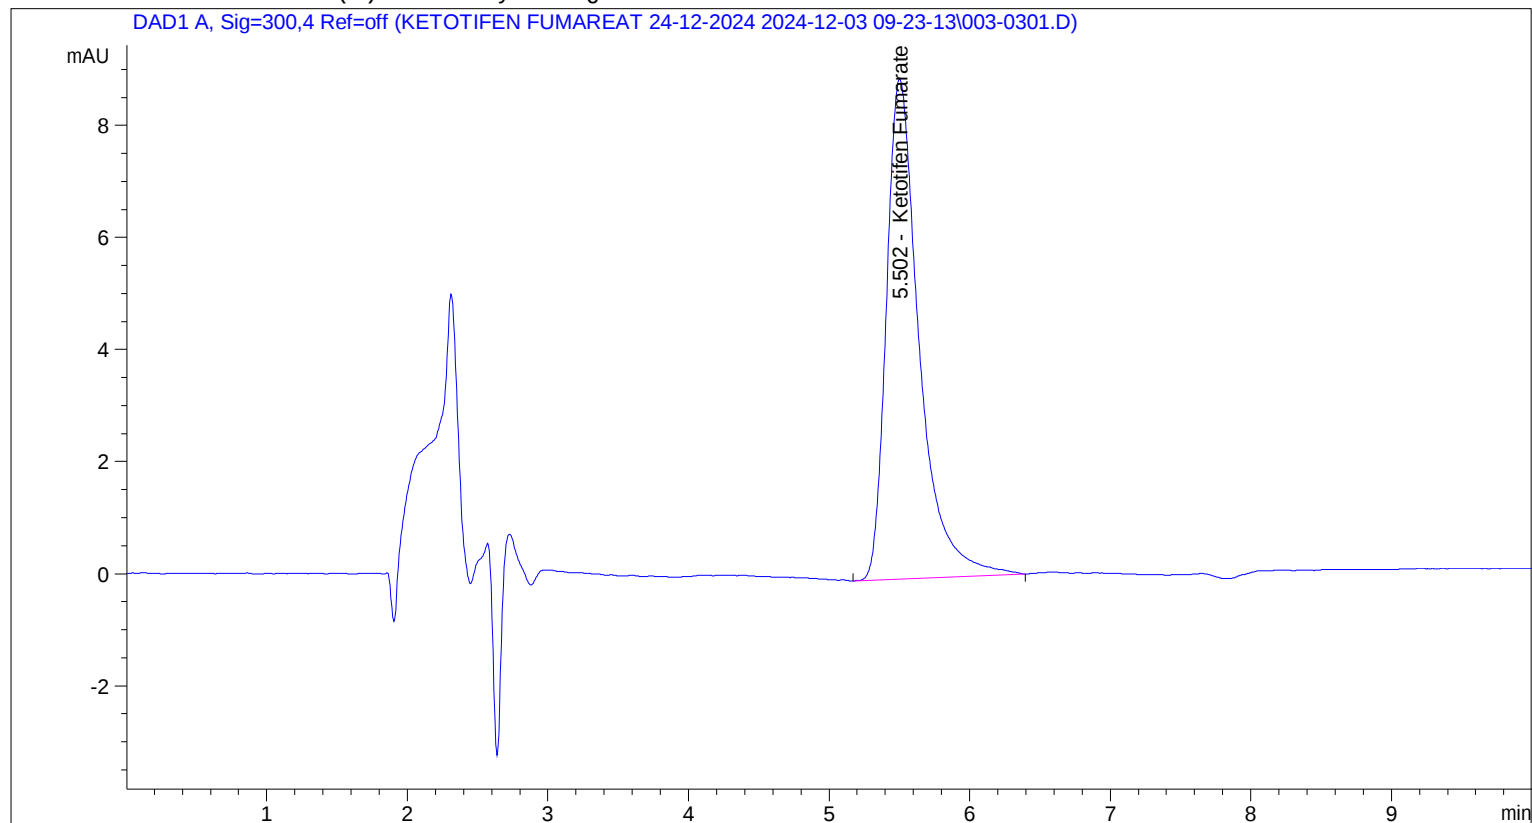

```

=====
                        Area Percent Report
=====
  
```

```

Sorted By      :      Signal
Calib. Data Modified : 12/4/2024 5:33:29 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=300,4 Ref=off

| Peak # | RetTime [min] | Type | Width [min] | Area [mAU*s] | Area %   | Name               |
|--------|---------------|------|-------------|--------------|----------|--------------------|
| 1      | 5.502         | BB   | 0.2411      | 144.71188    | 100.0000 | Ketotifen Fumarate |

Totals : 144.71188

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Invalid calibration curve, (Ketotifen Fumarate)

=====

\*\*\* End of Report \*\*\*