

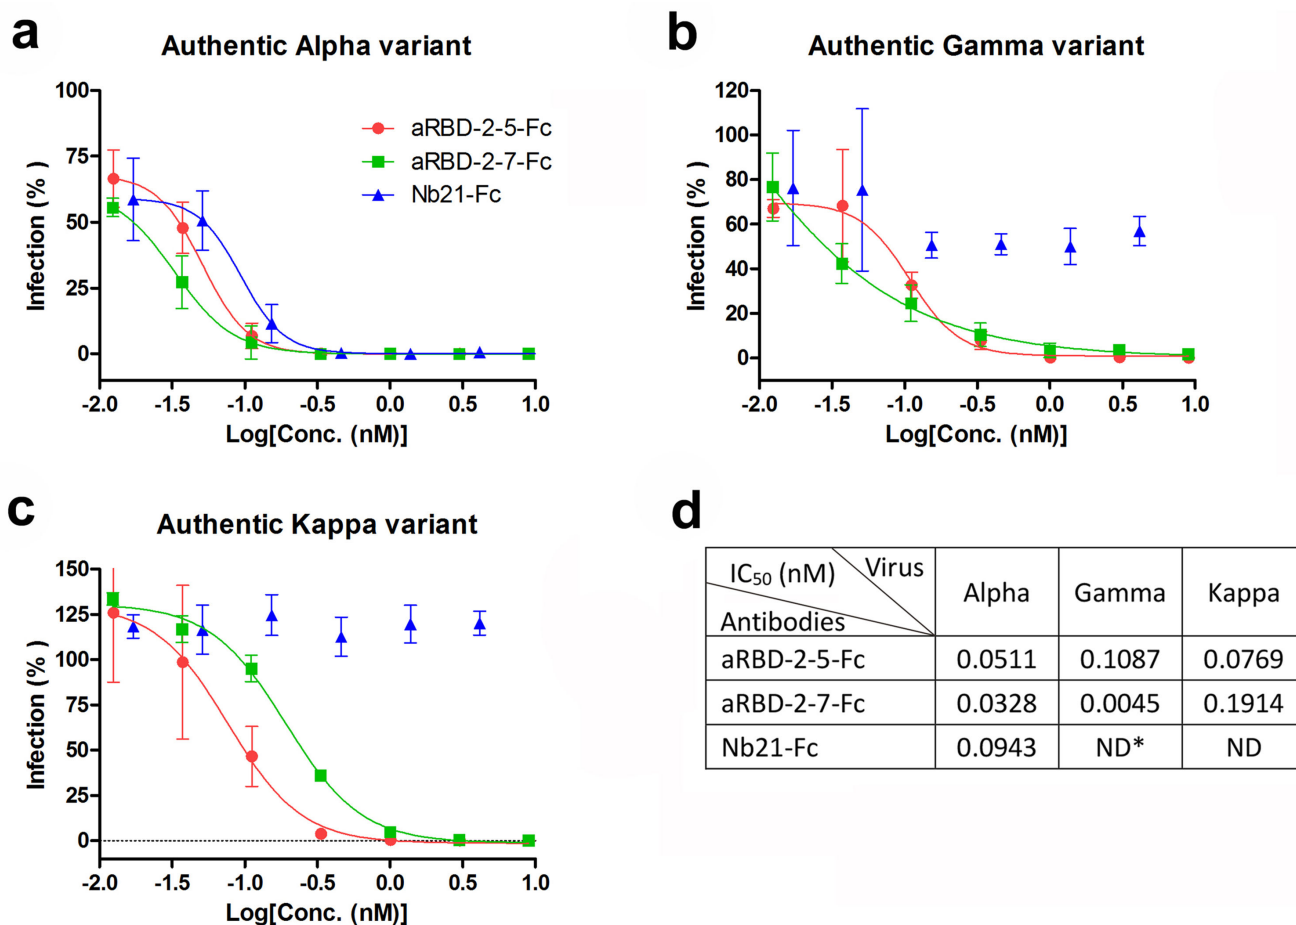


Fig. S10 Neutralization of authentic Alpha, Gamma and Kappa variants by aRBD-2-5-Fc and aRBD-2-7-Fc using microneutralization assay. Approximately 200 PFU of authentic Alpha (a), Gamma (b), and Kappa (c) variants were neutralized with serially diluted antibodies. Error bars indicate the mean $\pm$ SD from three independent experiments. IC₅₀ values were calculated by fitting the Infection (%) values of the serial dilution with a sigmoidal dose-response curve, and listed in (d). *ND, neutralization not detected.