

Supplementary information

**Nanofiber-Based Self-Adhesive Electrode Using
Self-Doped PEDOT and Polyurethane**

Ryota Fukuzawa, Chiaki Ushimaru, Kento Yamagishi, Hirokazu Yano,
Hidenori Okuzaki, Tomoyuki Yokota, and Takao Someya*

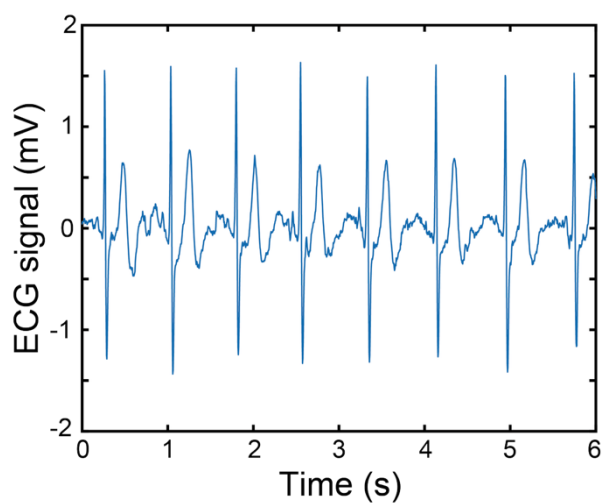


Figure S1 ECG signal taken on outside the sauna before entering and sweating in the sauna.

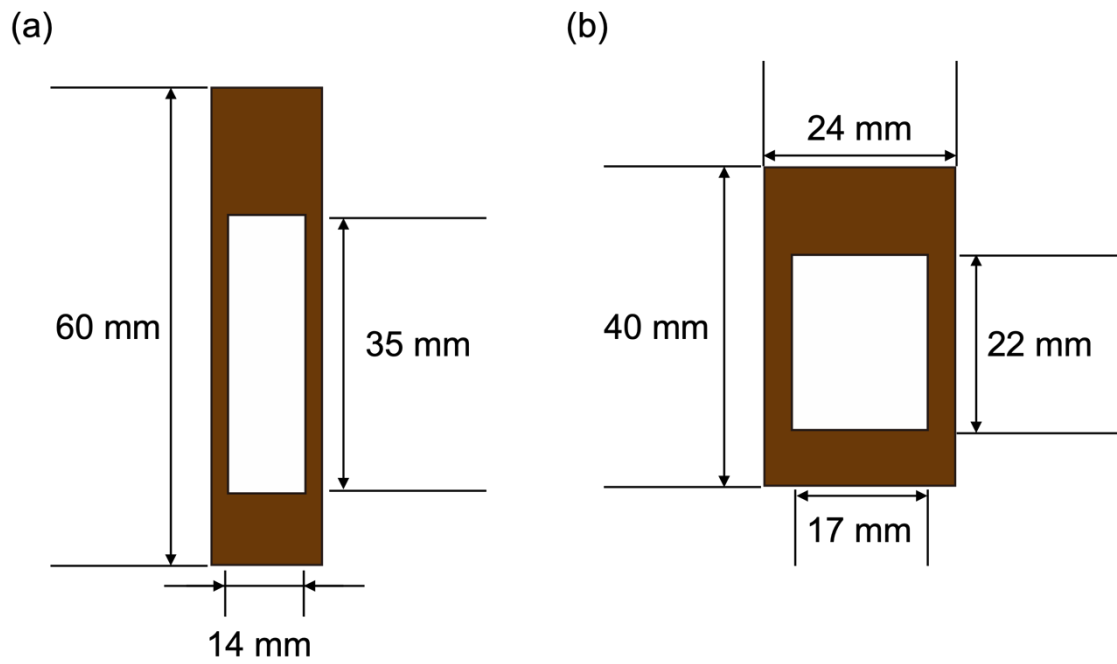


Figure S2 Schematic of the PI frames. The window sizes are (a) 35 mm $\times$ 14 mm and (b) 24 mm $\times$ 17 mm, respectively. The frame in (a) was used only for the four-terminal sensing method.

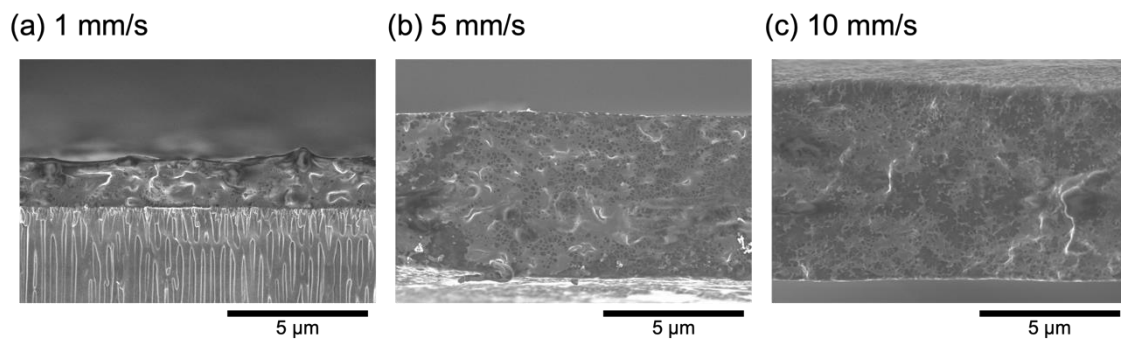


Figure S3 Cross-sectional SEM images at different withdrawal speeds in the dip-coating process. The speeds were (a) 1 mm/s, (b) 5 mm/s, and (c) 10 mm/s.