

Original Full Gel Picture

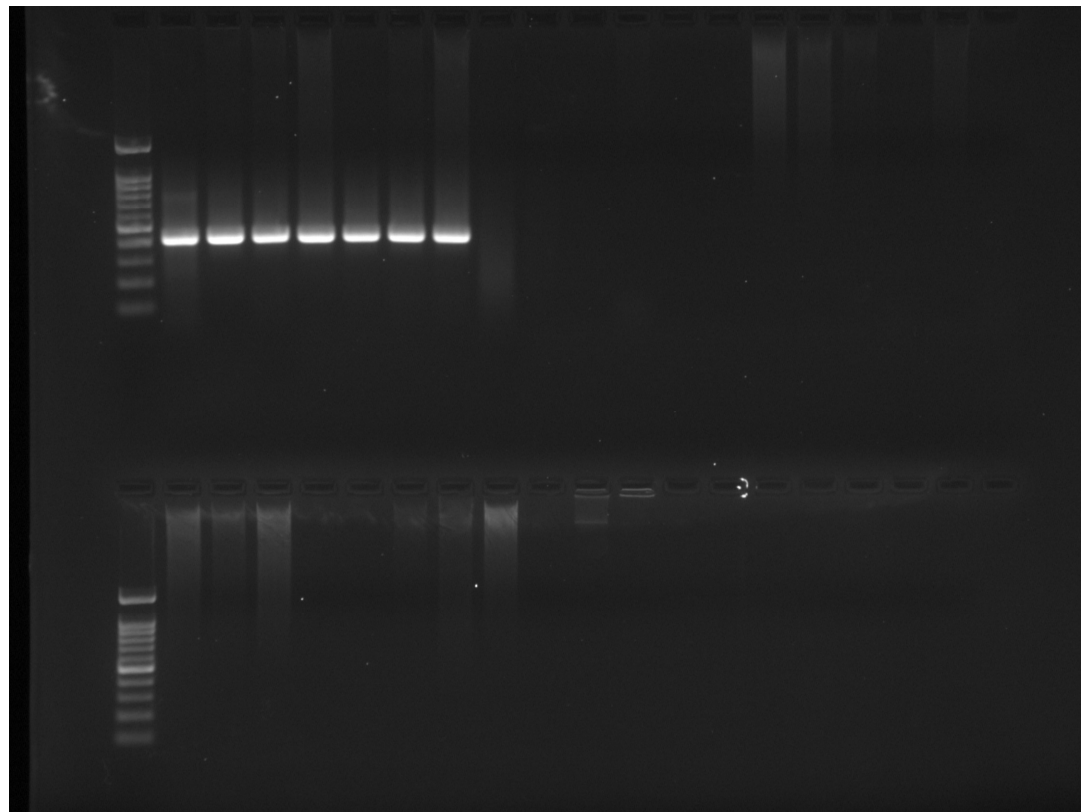


Figure 3. The specificity validation of the endpoint PCR primer pair designed to specifically detect *Dickeya fangzhongdai*.

Original Full Gel Picture

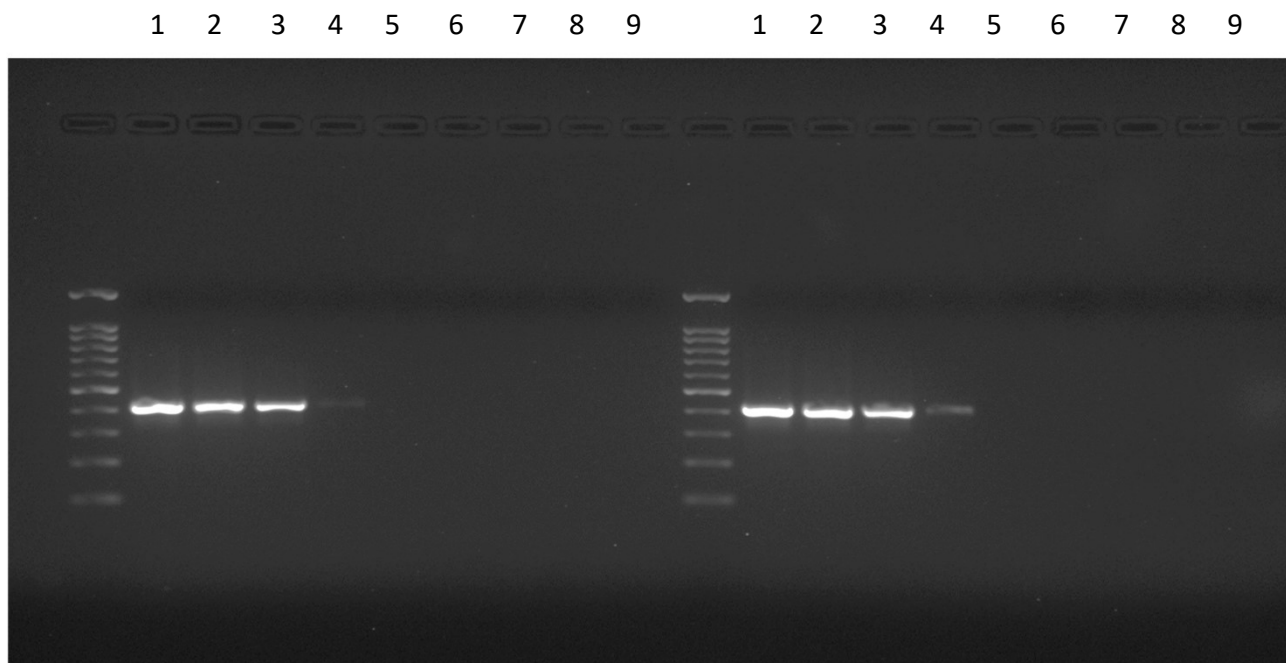


Figure 4. Detection limit determination of loop mediated isothermal amplification (LAMP) assay designed for specific detection of *Dickeya fangzhongdai*.
(D) Endpoint sensitivity assay with genomic DNA, serially diluted 10-fold (from 10 ng to 1 fg);
(E) spiked assay (1 μ l of healthy taro corm genomic DNA was added in 10-fold serially diluted genomic DNA).