


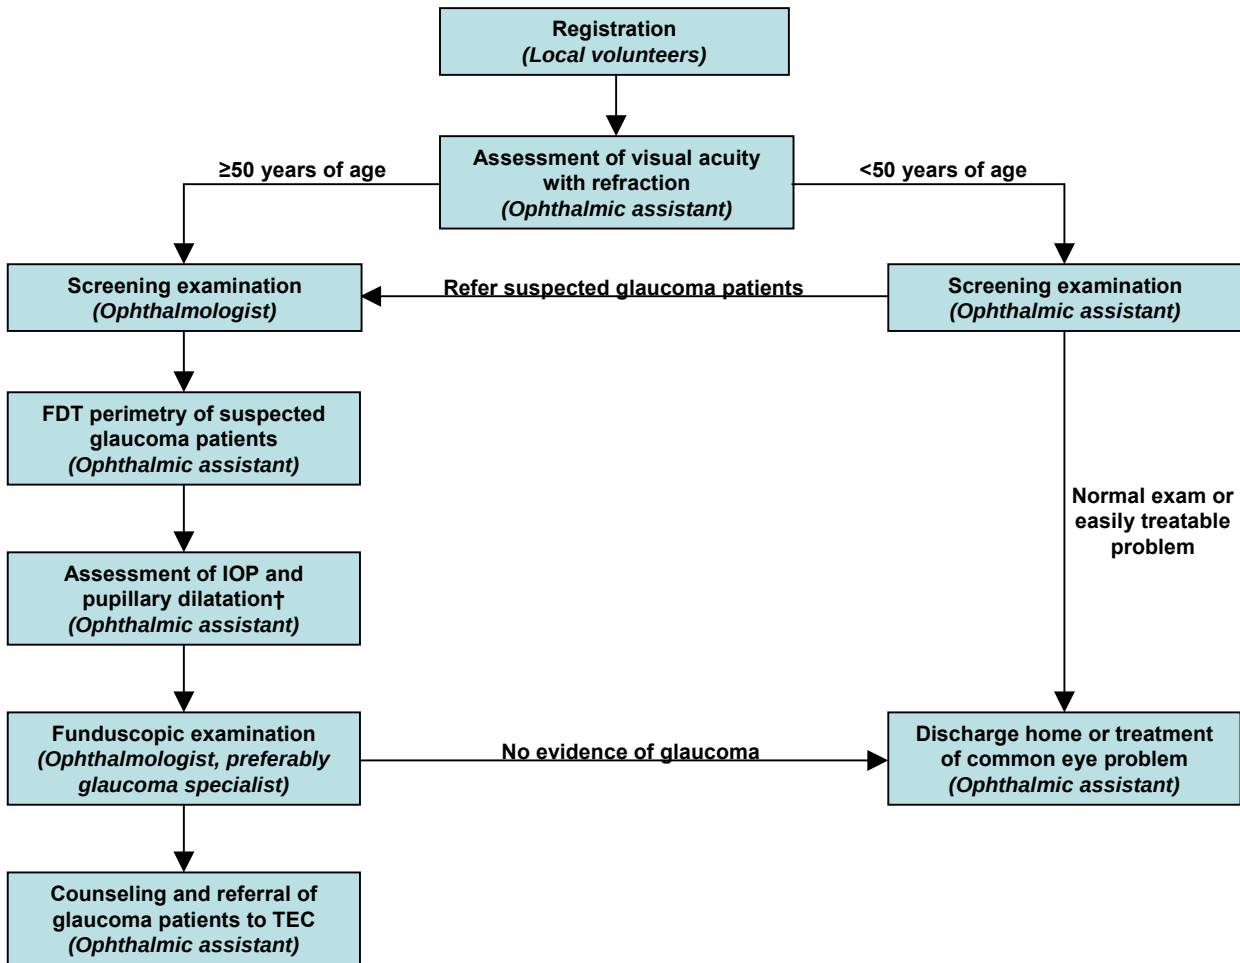

FDT=frequency doubling technology; IOP=intraocular pressure; TEC=Tilganga Eye Centre.

†Patients with shallow anterior chambers are referred to TEC for gonioscopy instead.