


Supplementary Figure 3 The calibration curve of our prediction model in the internal validation set.

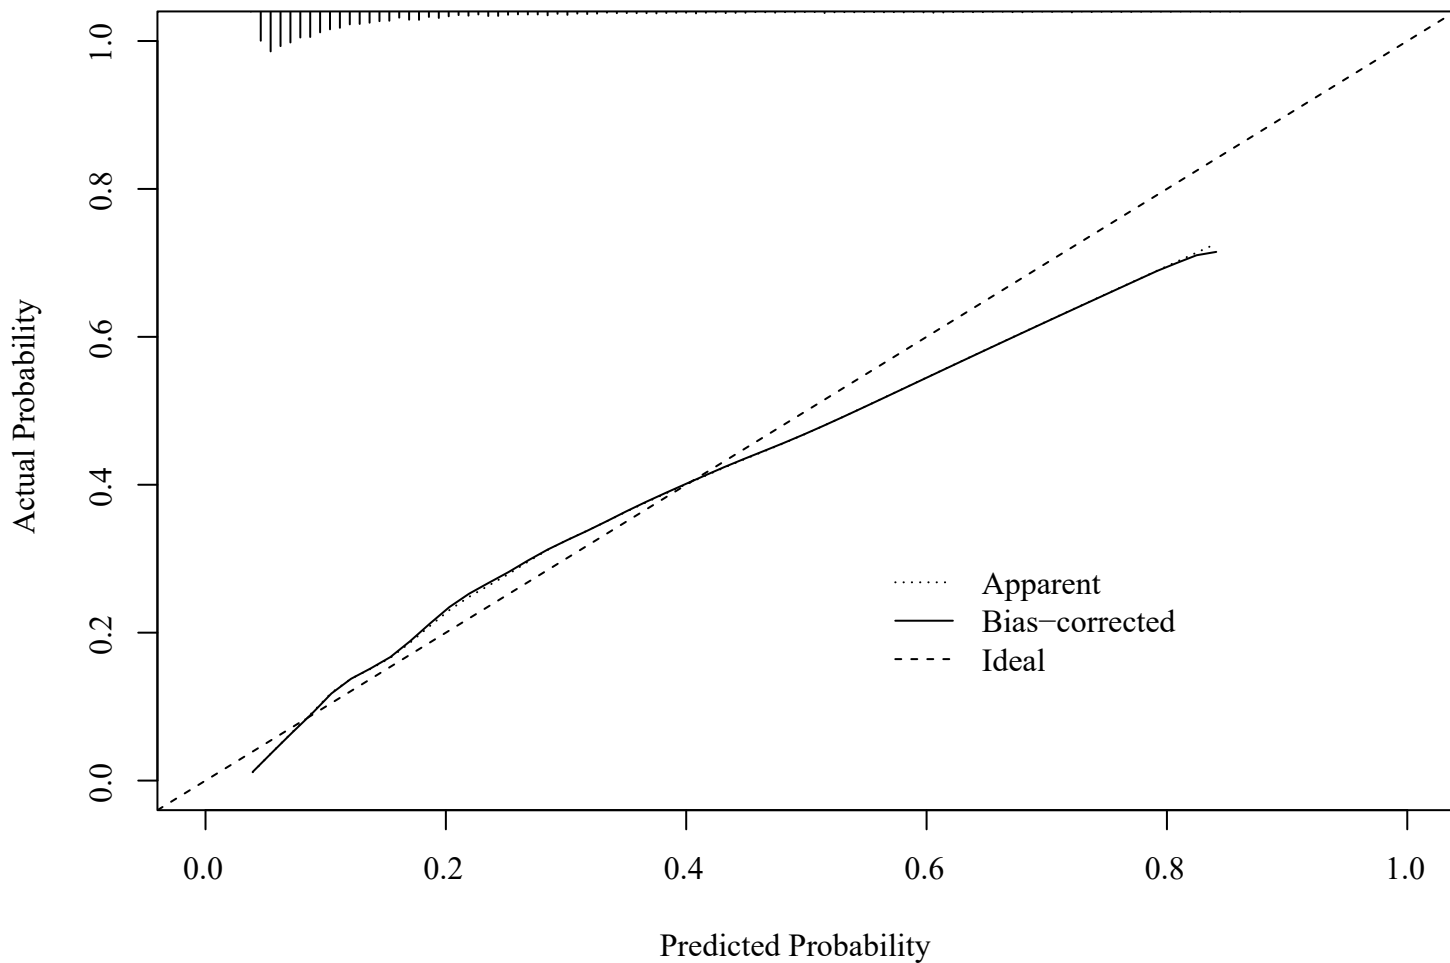

B= 40 repetitions, boot

Mean absolute error=0.018 n=4237