

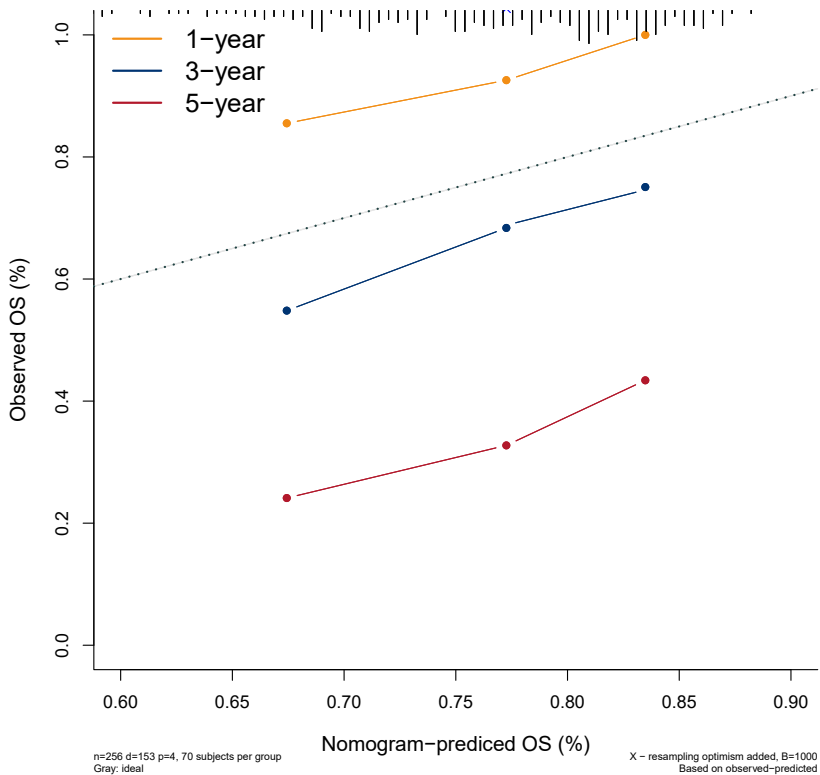


Figure S2. Calibration plot at 1-, 3-, and 5-year of nomogram without IPM.