


Additional files

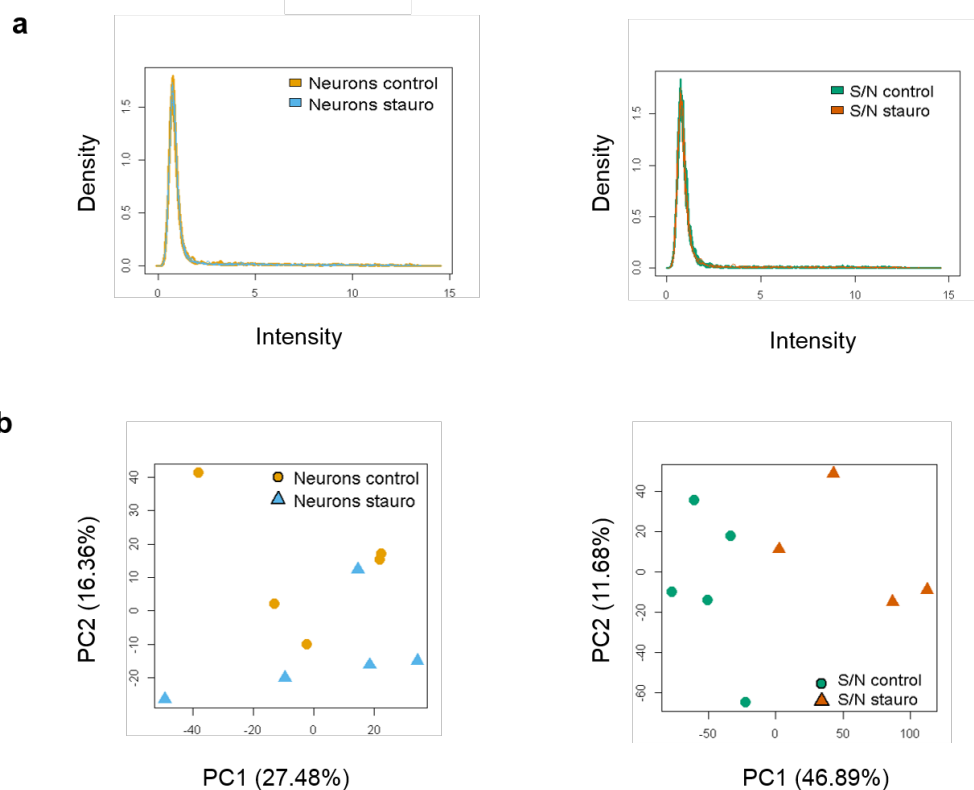

Additional file 1 Quality control parameter after normalization for mouse probes of the GeneChip miRNA array. Density histograms of probe intensities (**a**) and principal components analysis (**b**) for apoptotic cortical neurons and corresponding neuronal supernatant (S/N), as indicated, are shown.