

Fig. 1e


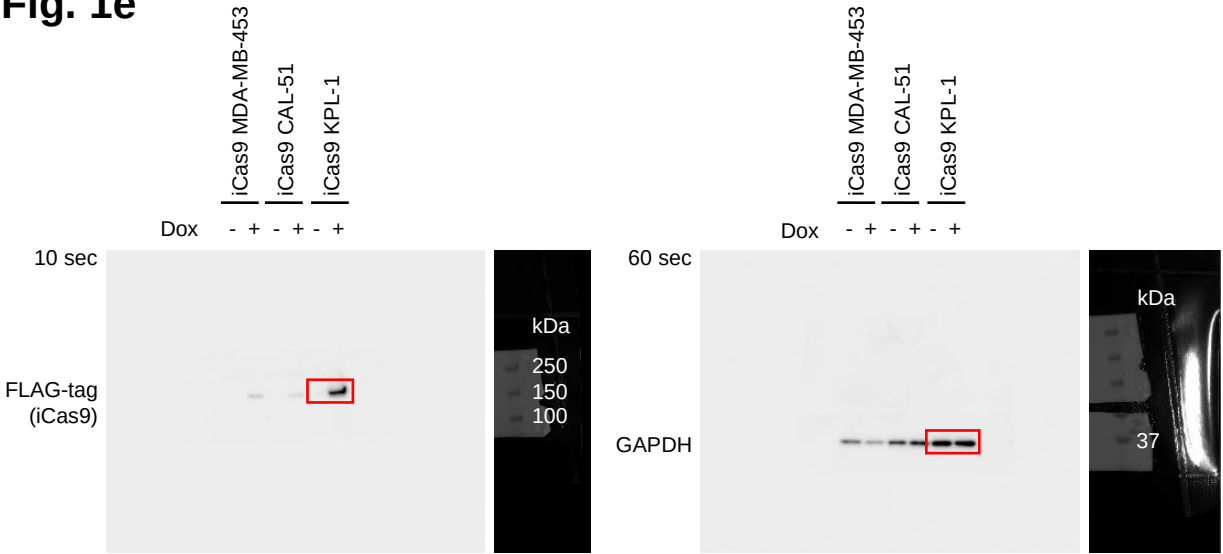


Fig. 1f

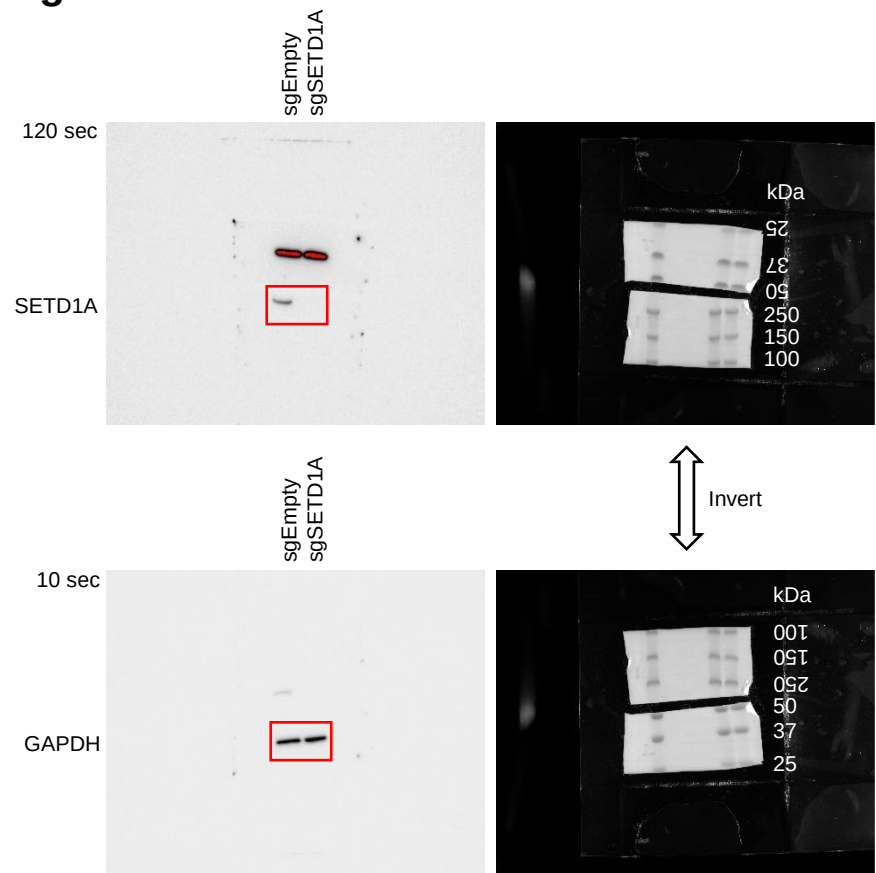

Due to an inadvertent mistake, one of the membranes was placed upside down during imaging. We acknowledge this issue and take full responsibility for it. However, we assure readers that the data presented in the manuscript are accurate.

Fig. 3a

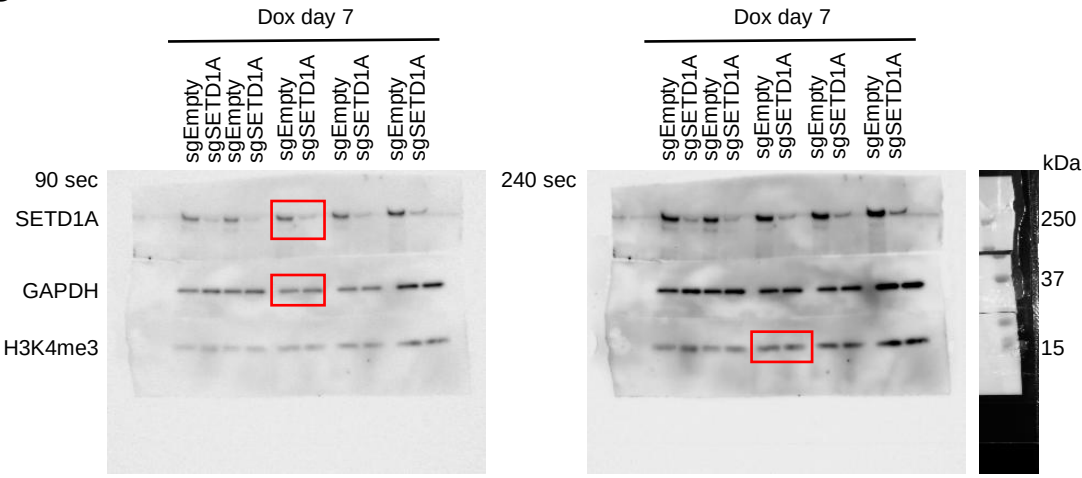


Fig. 3f

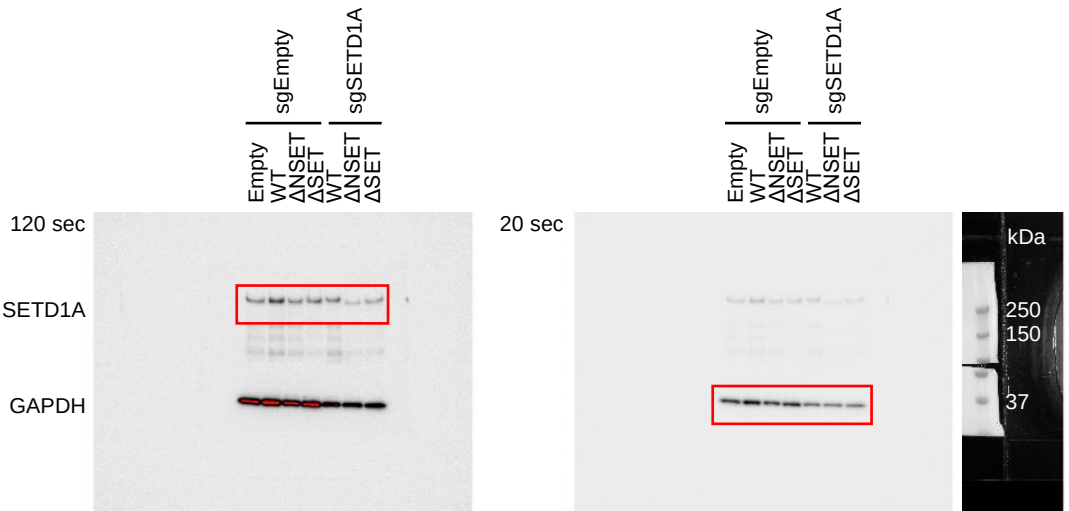


Fig. 4e

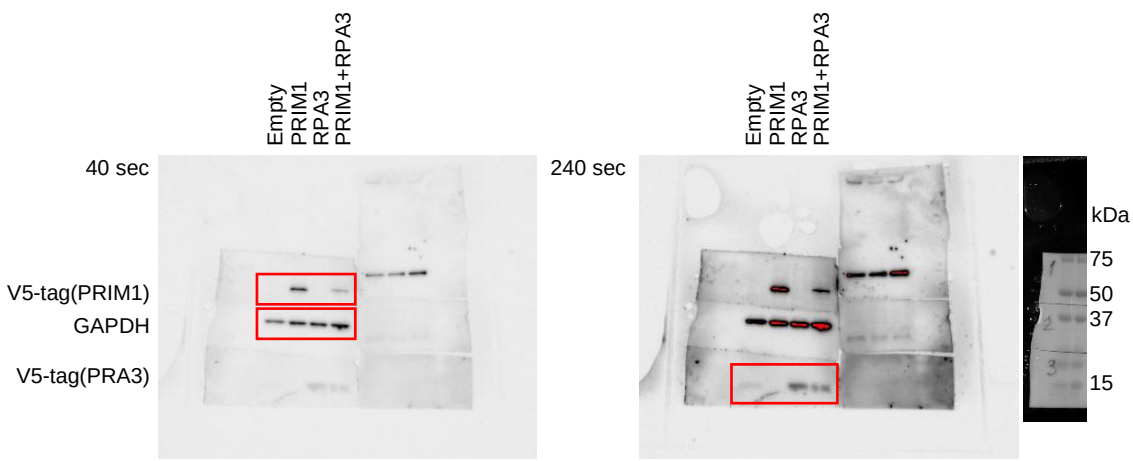


Fig. 6a

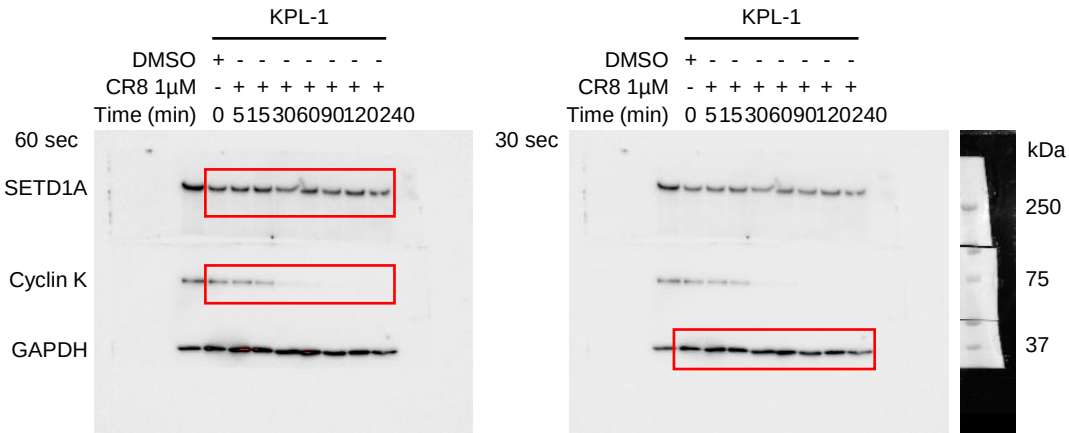


Fig. 6g, S6a, S6f

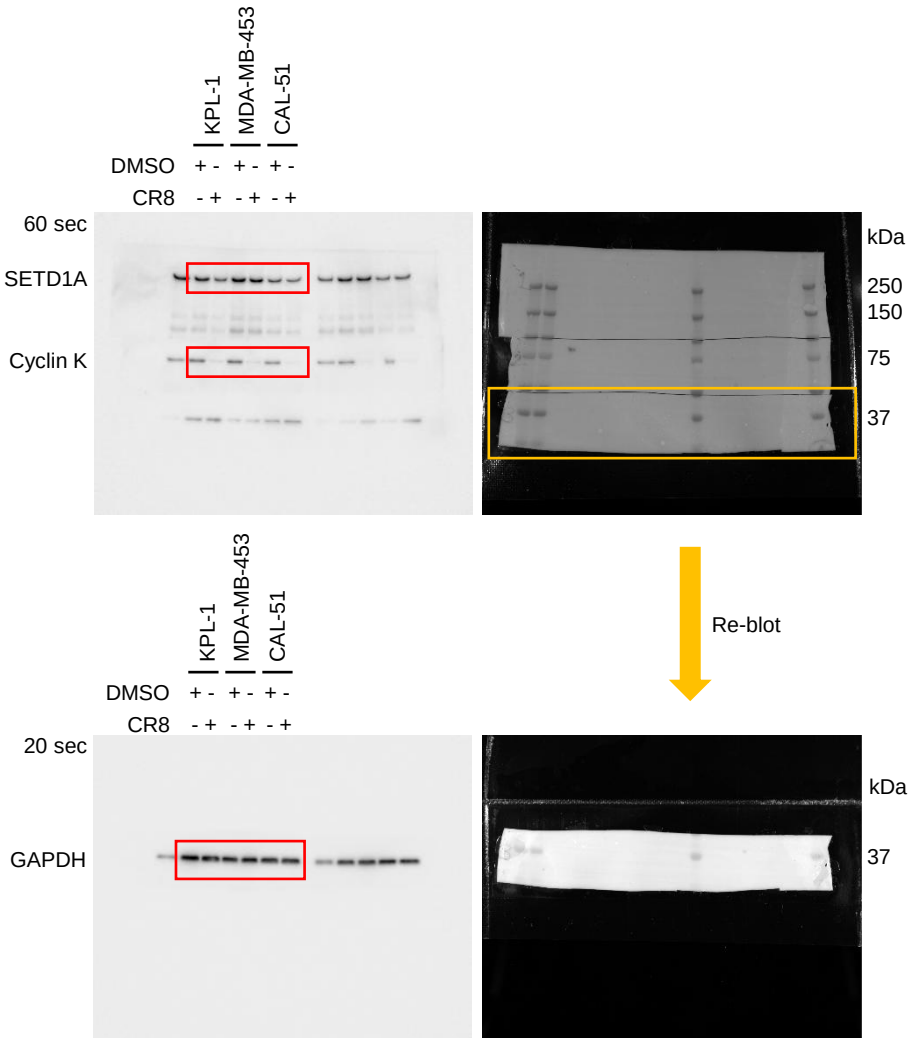


Fig. S1e

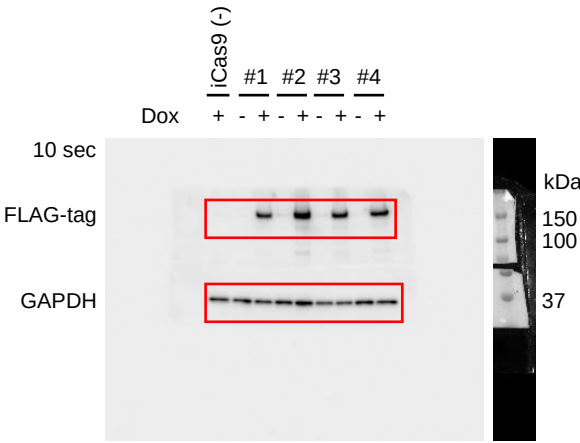


Fig. S4a

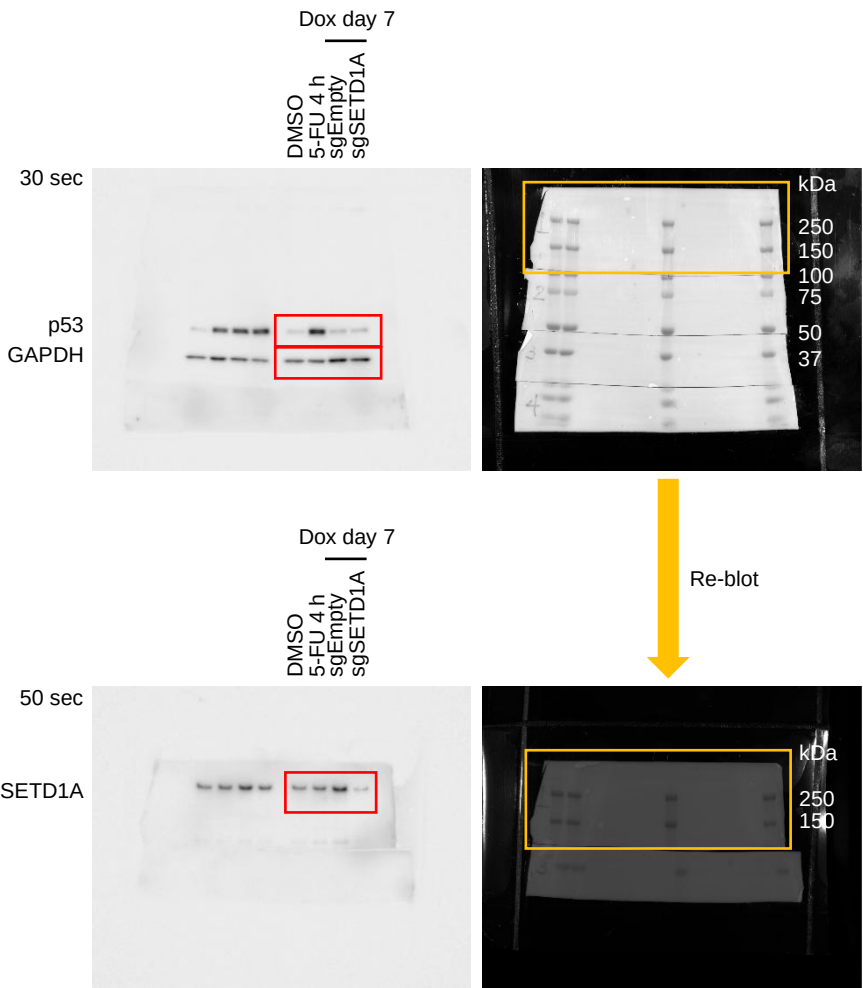


Fig. S4b

