


Anton Swart Biokinetic Rehabilitation Practice

Name: 001 001 001
Number: 001
Gender: Male
Birthdate: 01/06/1967 50 years

Recorded: 06/05/2018 07:17:48
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

P / PQ: 107 ms / 152 ms
QRS: 80 ms
QT / QTc / QTd: 406 ms / 441 ms / -
P/QRS/T axis: 72° / 81° / 68°
Heartrate: 80 bpm

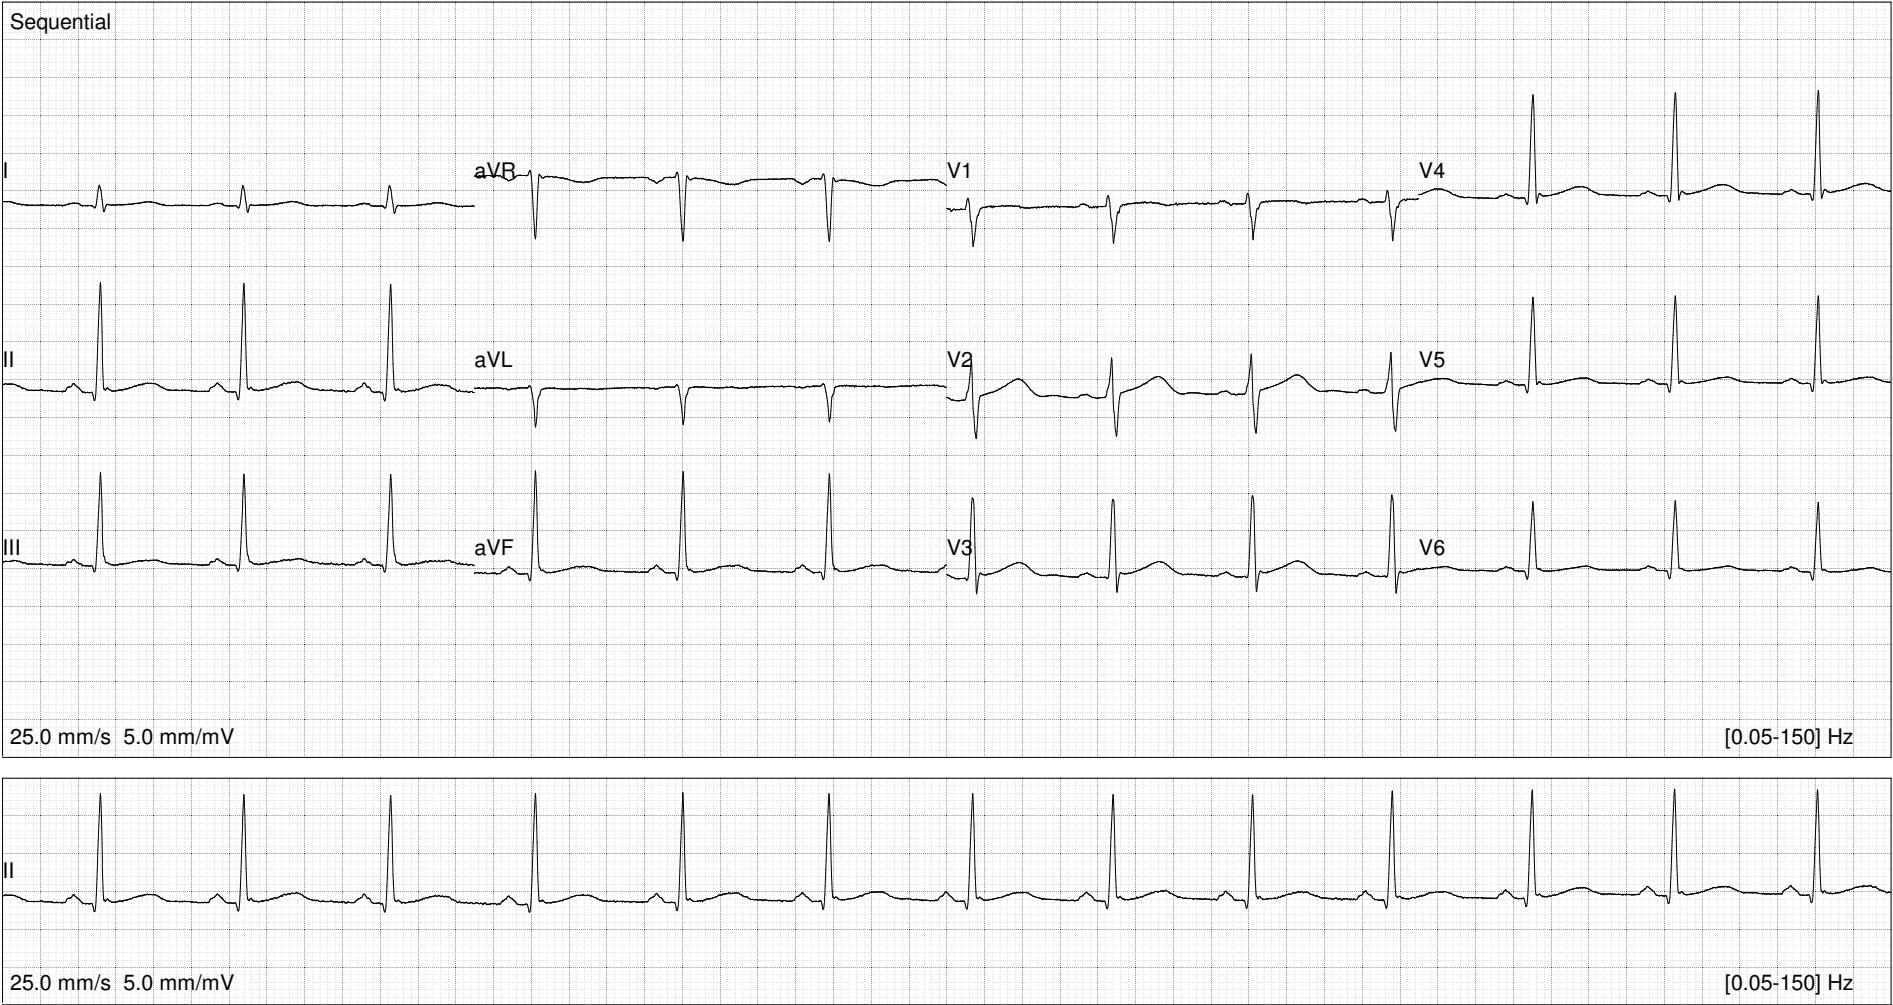

Anton Swart Biokinetic Rehabilitation Practice

Name:

001 001 001

Number:

001

Gender:

Male

Birthdate:

01/06/1967 50 years

P / PQ:

107 ms / 152 ms

QRS:

80 ms

QT / QTc / QTd:

406 ms / 441 ms / -

P/QRS/T axis:

72° / 81° / 68°

Heartrate:

80 bpm

Recorded:

06/05/2018 07:17:48

Recorded by:

Mr. Anton Swart

Referring physician:

Location:

Anton Swart Biokinetic Rehabilitation Practice



Ordering physician:

Attending physician:

Comment:




UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	396	Minimum	700 ms
Normal:	396	Maximum	820 ms
Other:	0	Mean:	756 ms
		SD:	18 ms

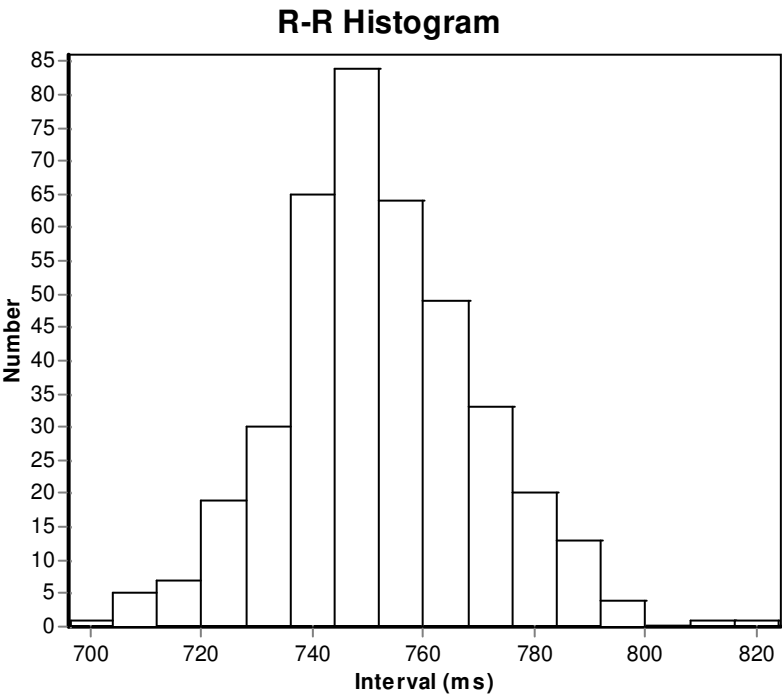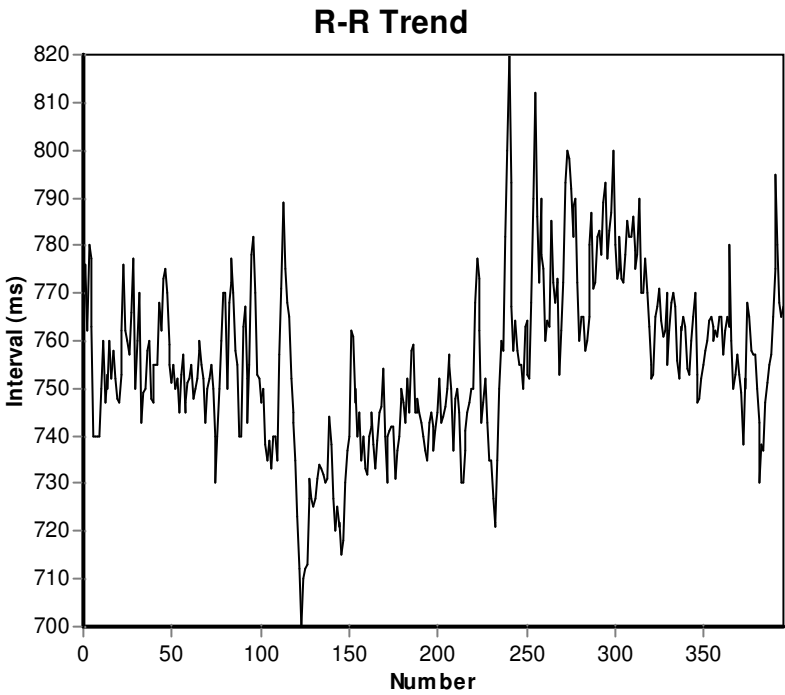

Heart Rate Variability: Time Domain Analysis

Name: 001, 001 001 Birthdate: 01/06/1967
 Number: 001 Recorded: 06/05/2018 07:17:48
 Gender: Male

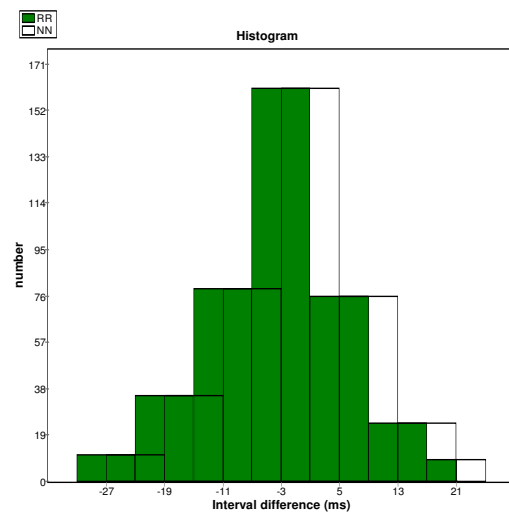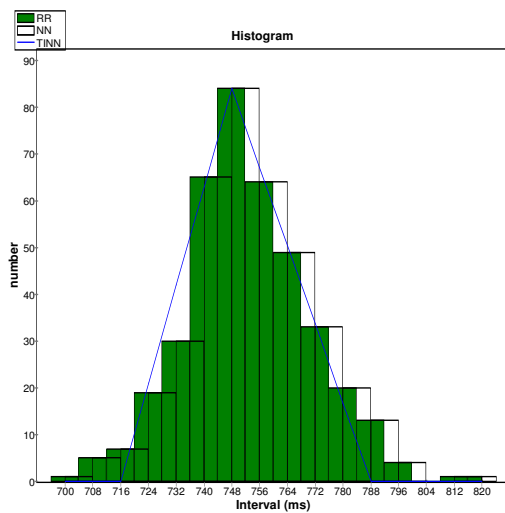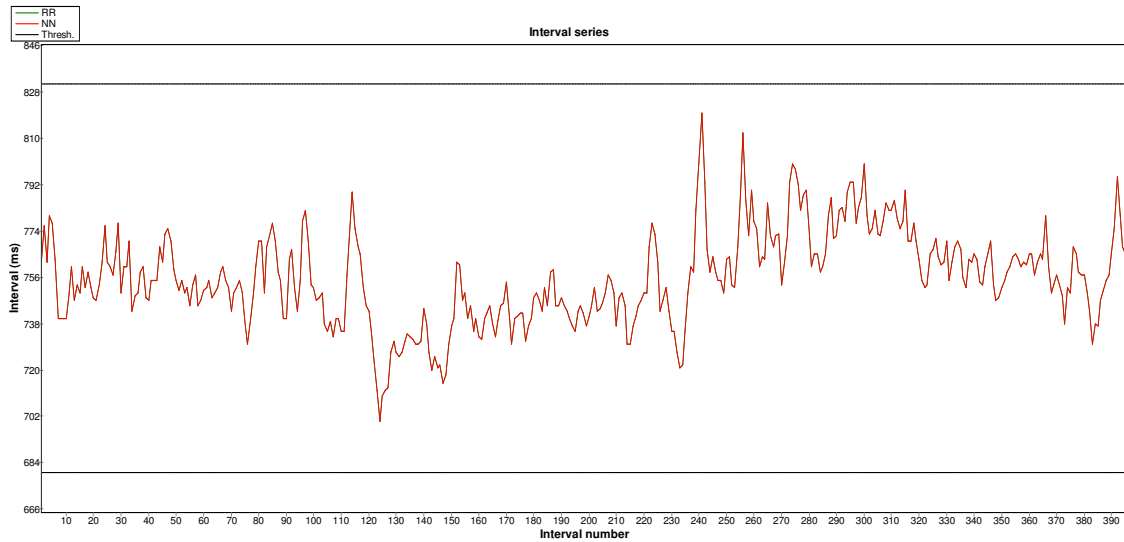

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	18	18
Triangular Interpolation (ms)	72	72
Triangular Index	4.71	4.71

HRV parameters	NN	RR
SDSD (ms)	9	9
RMSSD (ms)	9	9
NN50	0	0
NN50(1)	0	0
NN50(2)	0	0
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	1.24	1.24
SD(Logarithmic Index)	0.13	0.13



Interval statistics	NN	RR
Number	396	396
Minimum (ms)	700	700
Maximum (ms)	820	820
Range (ms)	120	120
Avg (ms)	756	756
SD (ms)	18	18
AvgDev (ms)	14	14
p5 (ms)	727	727
p50 (ms)	755	755
p95 (ms)	788	788
Skewness	0.20	0.20
Kurtosis	3.38	3.38

Interval statistics	NN	RR
Number	395	395
Minimum (ms)	-27	-27
Maximum (ms)	24	24
Range (ms)	51	51
Avg (ms)	0	0
SD (ms)	9	9
AvgDev (ms)	7	7
p5 (ms)	-15	-15
p50 (ms)	1	1
p95 (ms)	17	17
Skewness	-0.12	-0.12
Kurtosis	3.33	3.33

Heart Rate Variability: Frequency Domain Analysis

Name: 001, 001 001
Number: 001
Gender: Male

Birthdate: 01/06/1967
Recorded: 06/05/2018 07:17:48

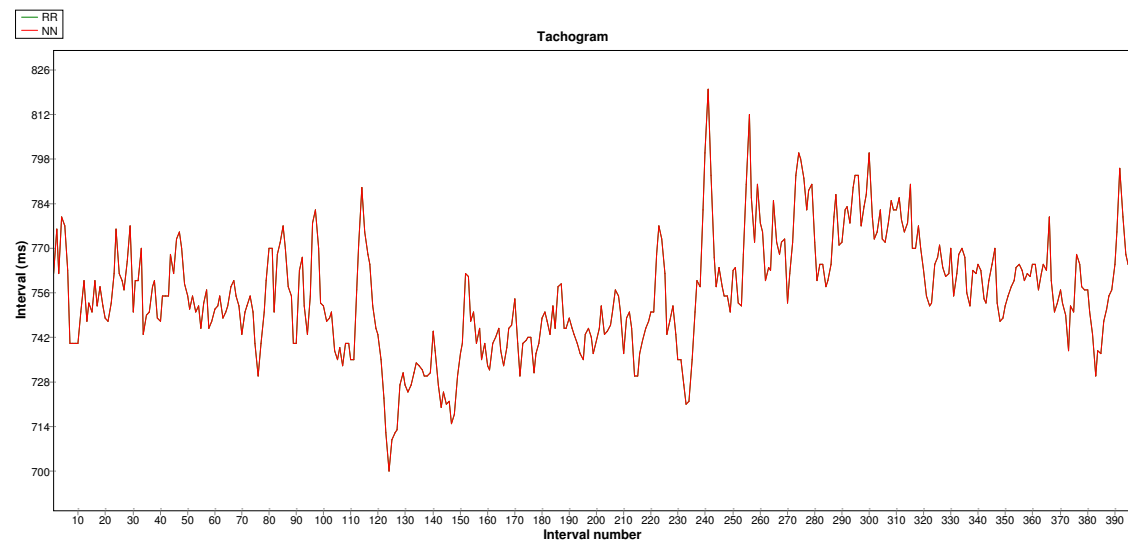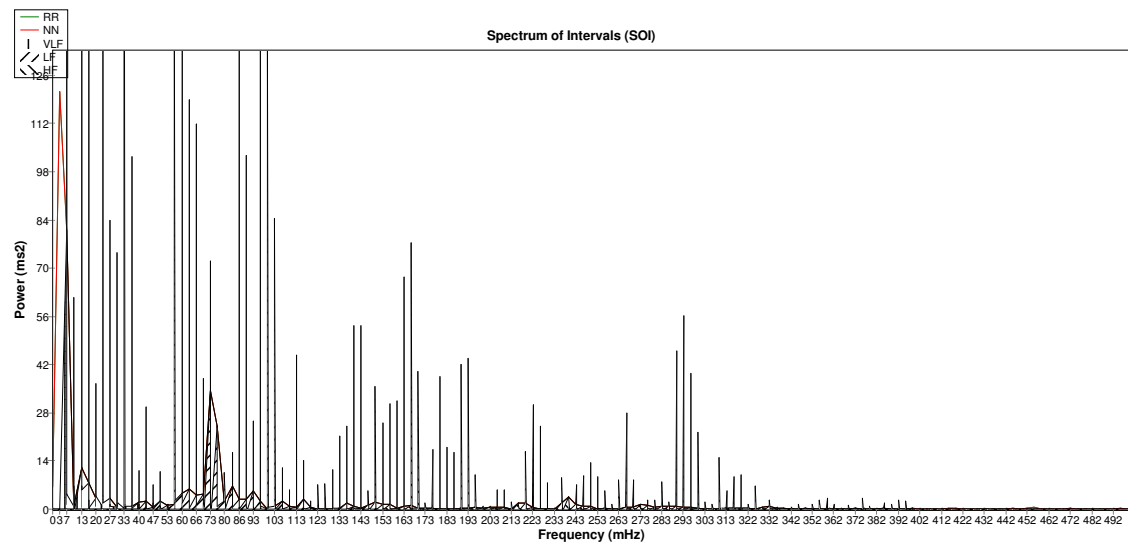

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	273	273	Spectrum of Intervals (SOI)	
VLF (ms2)	113	113	Frequency resolution (mHz)	3
LF (ms2)	123	123	VLF lower boundary (mHz)	3
HF (ms2)	37	37	VLF upper boundary (mHz)	40
LF/HF	3.37	3.37	LF upper boundary (mHz)	150
LF normalized	77.10	77.10	HF upper boundary (mHz)	400
HF normalized	22.90	22.90	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	73	73	Fourier transform	DFT
HF peak (mHz)	239	239	Sample frequency (Hz)	1.32
			Interval correction	Annotation
			Interval threshold (%)	10