


Anton Swart Biokinetic Rehabilitation Practice

Name: 004 004 004
Number: 004
Gender: Male
Birthdate: 13/11/1964 53 years

Recorded: 03/05/2018 17:00:07
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

P / PQ: 115 ms / 157 ms
QRS: 110 ms
QT / QTc / QTd: 405 ms / 438 ms / -
P/QRS/T axis: 71° / 82° / 74°
Heartrate: 79 bpm

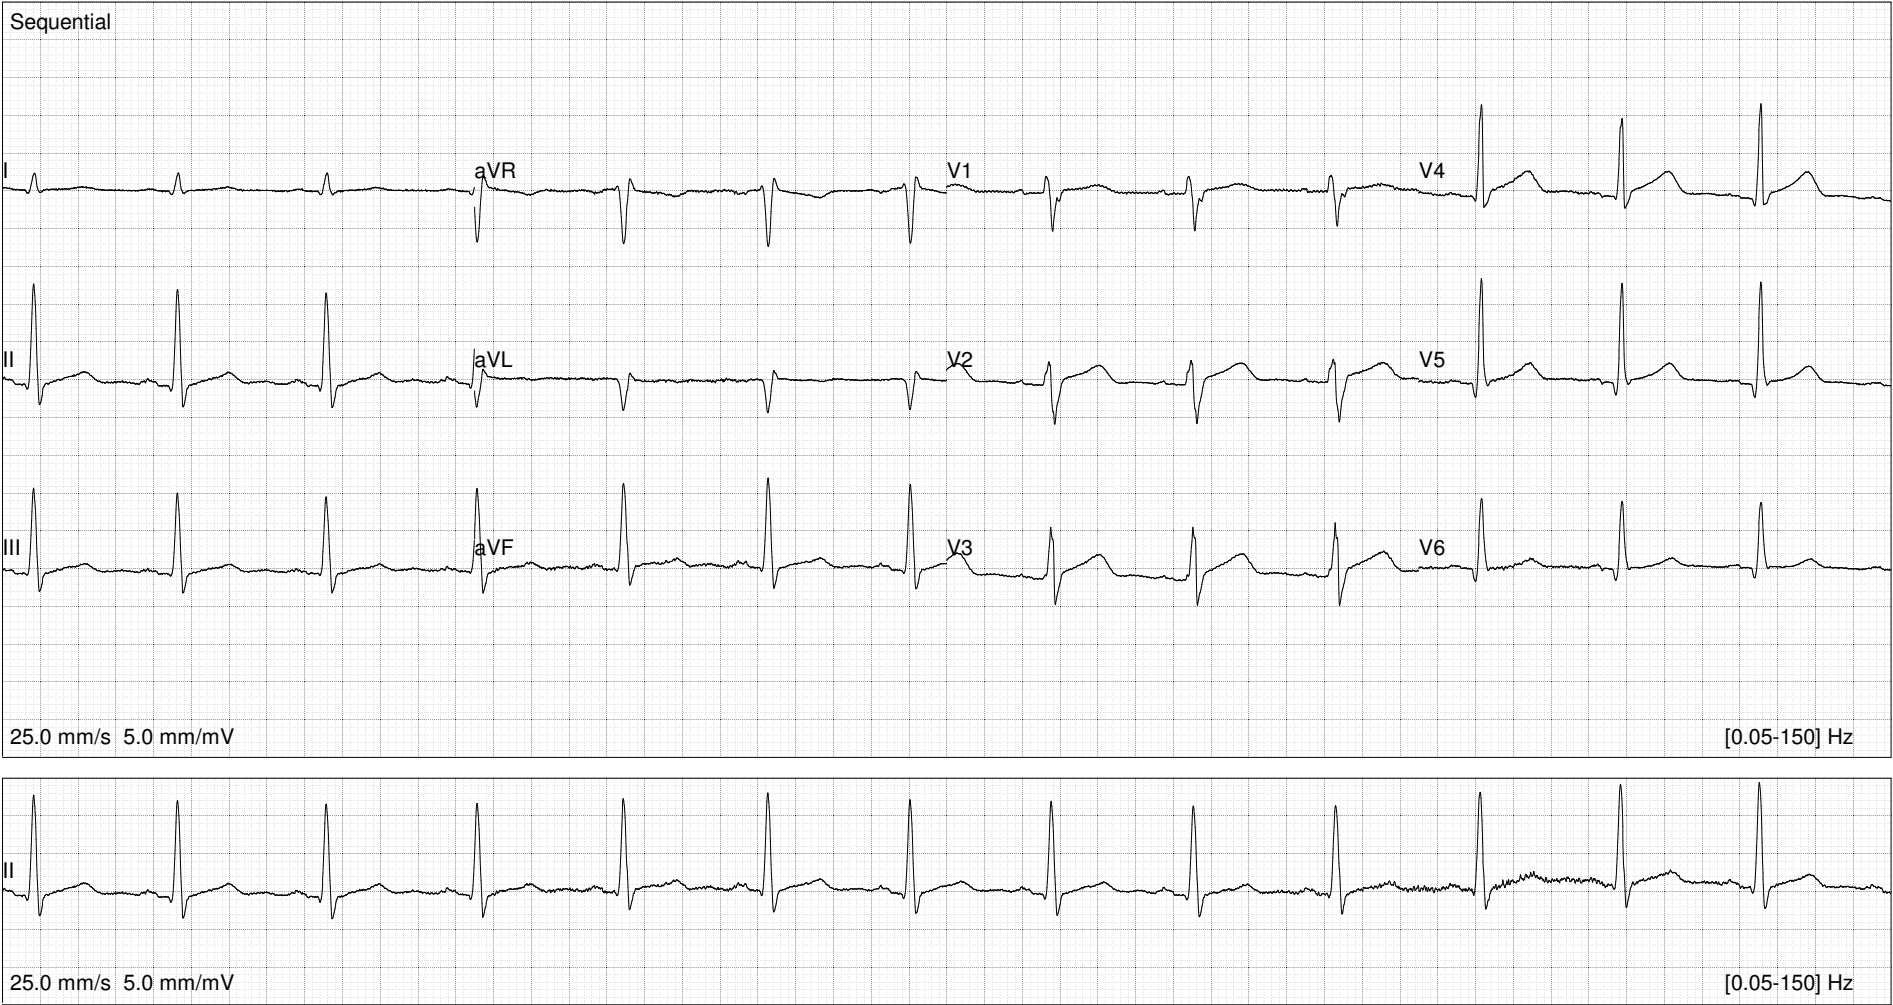

Anton Swart Biokinetic Rehabilitation Practice

Name: 004 004 004
Number: 004
Gender: Male
Birthdate: 13/11/1964 53 years


P / PQ: 115 ms / 157 ms
QRS: 110 ms
QT / QTc / QTd: 405 ms / 438 ms / -
P/QRS/T axis: 71° / 82° / 74°
Heartrate: 79 bpm

Recorded: 03/05/2018 17:00:07
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:


UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	394	Minimum	699 ms
Normal:	394	Maximum	814 ms
Other:	0	Mean:	760 ms
		SD:	20 ms

R-R Trend

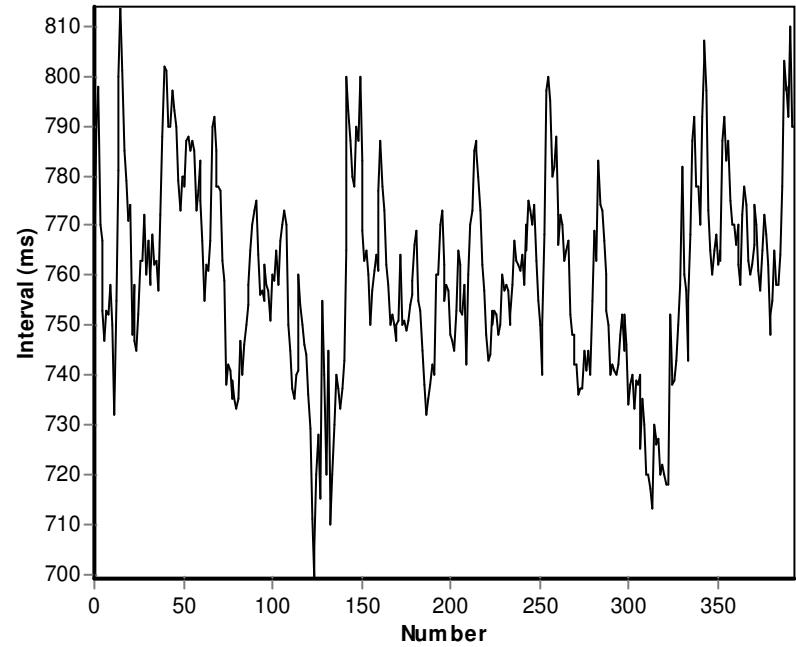



R-R Histogram

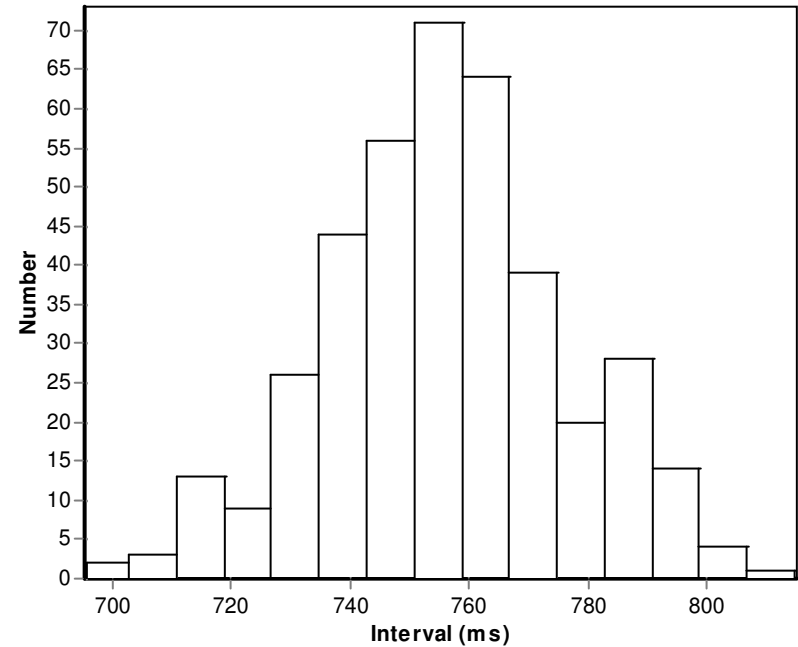

Heart Rate Variability: Time Domain Analysis

Name: 004, 004 004
Number: 004
Gender: Male


Birthdate: 13/11/1964
Recorded: 03/05/2018 17:00:07

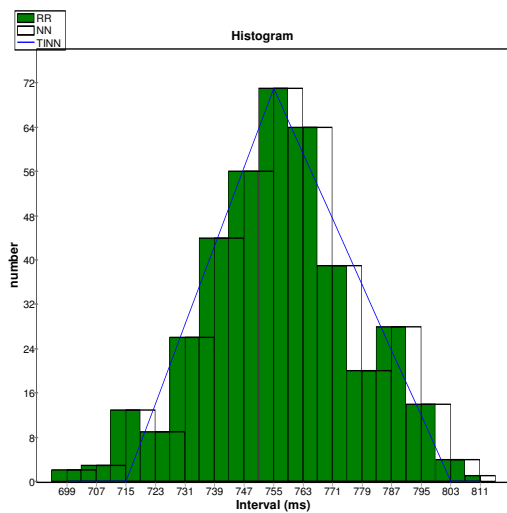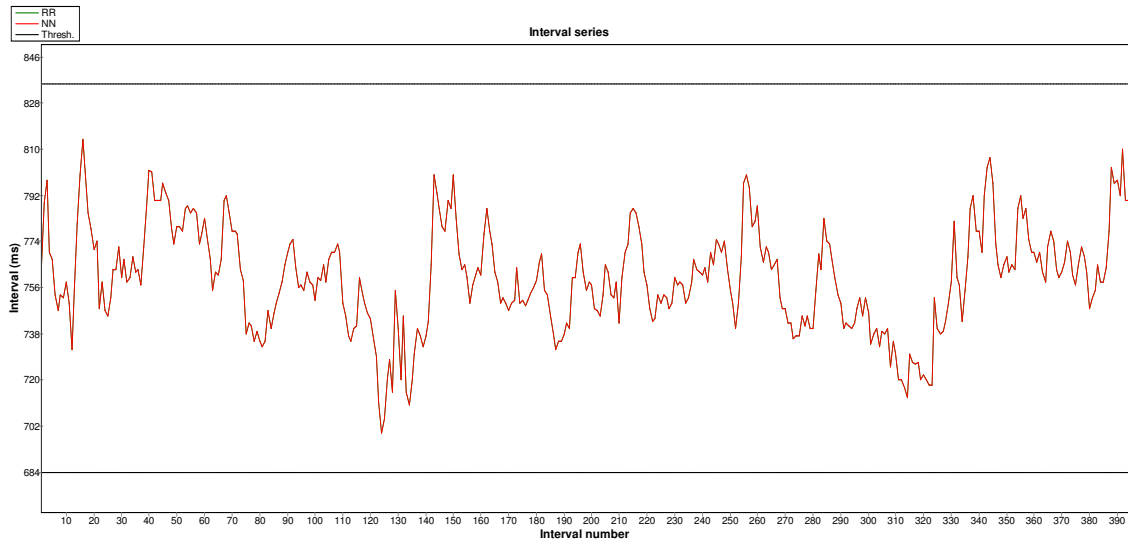

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	20	20
Triangular Interpolation (ms)	88	88
Triangular Index	5.55	5.55

Interval statistics	NN	RR
Number	394	394
Minimum (ms)	699	699
Maximum (ms)	814	814
Range (ms)	115	115
Avg (ms)	760	760
SD (ms)	20	20
AvgDev (ms)	16	16
p5 (ms)	726	726
p50 (ms)	760	760
p95 (ms)	794	794
Skewness	-0.02	-0.02
Kurtosis	2.96	2.96


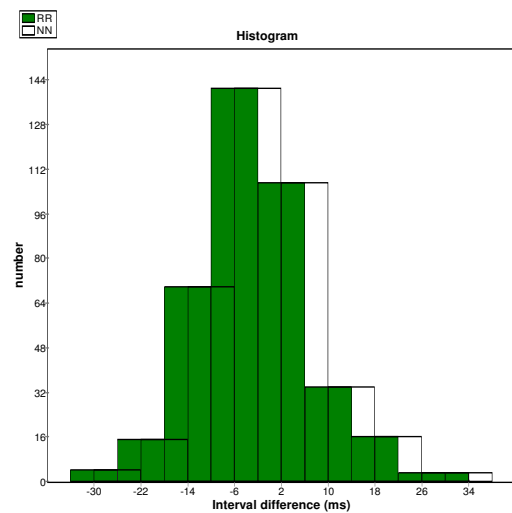


HRV parameters	NN	RR
SDSD (ms)	10	10
RMSSD (ms)	10	10
NN50	0	0
NN50(1)	0	0
NN50(2)	0	0
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	1.15	1.15
SD(Logarithmic Index)	0.05	0.05

Interval statistics	NN	RR
Number	393	393
Minimum (ms)	-30	-30
Maximum (ms)	40	40
Range (ms)	70	70
Avg (ms)	0	0
SD (ms)	10	10
AvgDev (ms)	7	7
p5 (ms)	-14	-14
p50 (ms)	-1	-1
p95 (ms)	19	19
Skewness	0.52	0.52
Kurtosis	4.45	4.45

Heart Rate Variability: Frequency Domain Analysis

Name: 004, 004 004 Birthdate: 13/11/1964
 Number: 004 Recorded: 03/05/2018 17:00:07
 Gender: Male

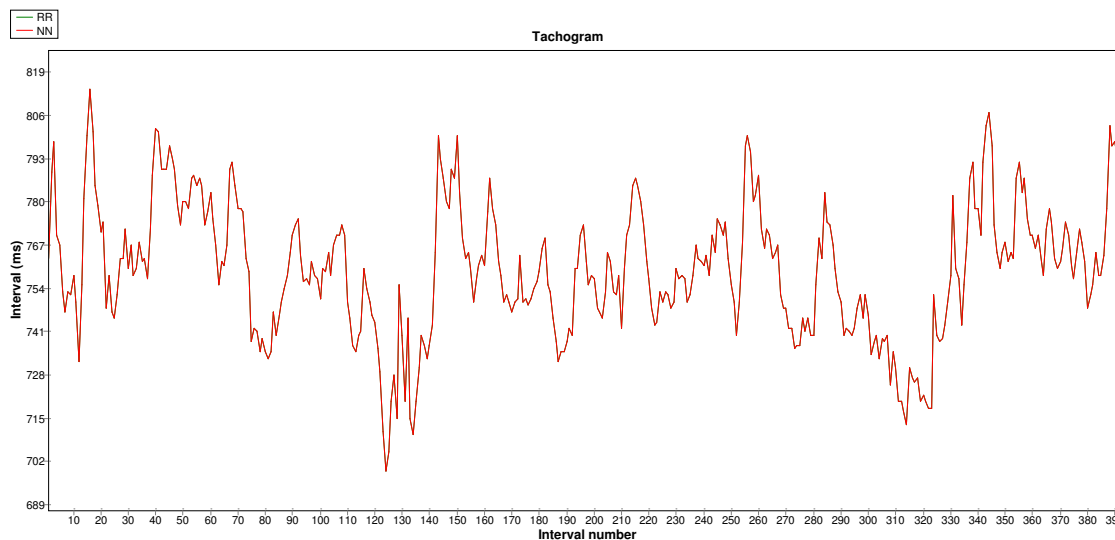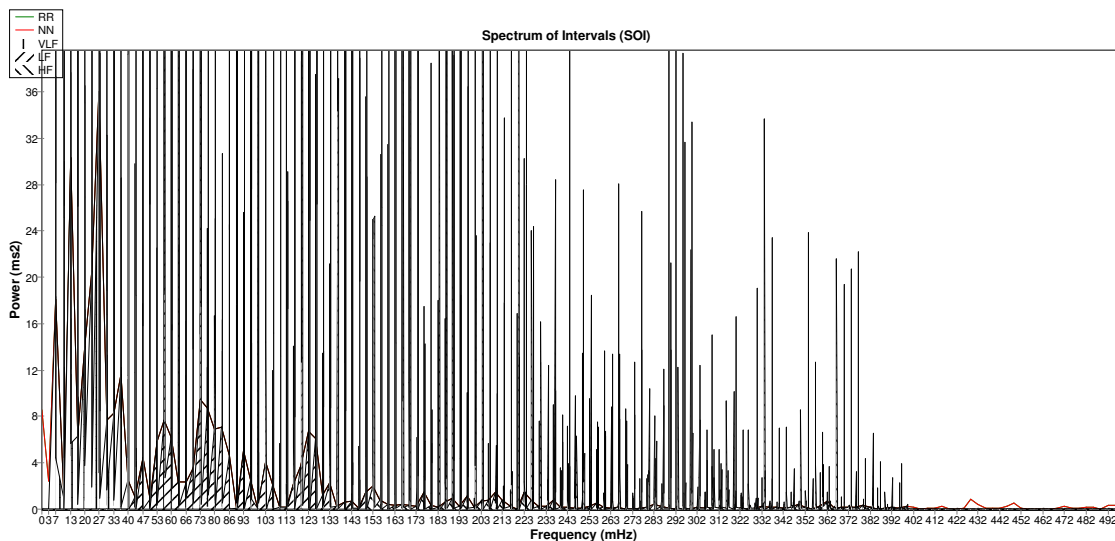

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	292	292	Spectrum of Intervals (SOI)	
VLF (ms2)	156	156	Frequency resolution (mHz)	3
LF (ms2)	111	111	VLF lower boundary (mHz)	3
HF (ms2)	25	25	VLF upper boundary (mHz)	40
LF/HF	4.49	4.49	LF upper boundary (mHz)	150
LF normalized	81.78	81.78	HF upper boundary (mHz)	400
HF normalized	18.22	18.22	Smoothing factor	1
VLF peak (mHz)	27	27	Tapering	Hann
LF peak (mHz)	73	73	Fourier transform	DFT
HF peak (mHz)	153	153	Sample frequency (Hz)	1.32
			Interval correction	Annotation
			Interval threshold (%)	10