


Anton Swart Biokinetic Rehabilitation Practice

Name: 004 004 004
Number: 004
Gender: Male
Birthdate: 13/11/1964 53 years

P / PQ: 113 ms / 143 ms
QRS: 109 ms
QT / QTc / QTd: 404 ms / 453 ms / -
P/QRS/T axis: 71° / 81° / 78°
Heartrate: 88 bpm

Recorded: 05/05/2018 12:18:48
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

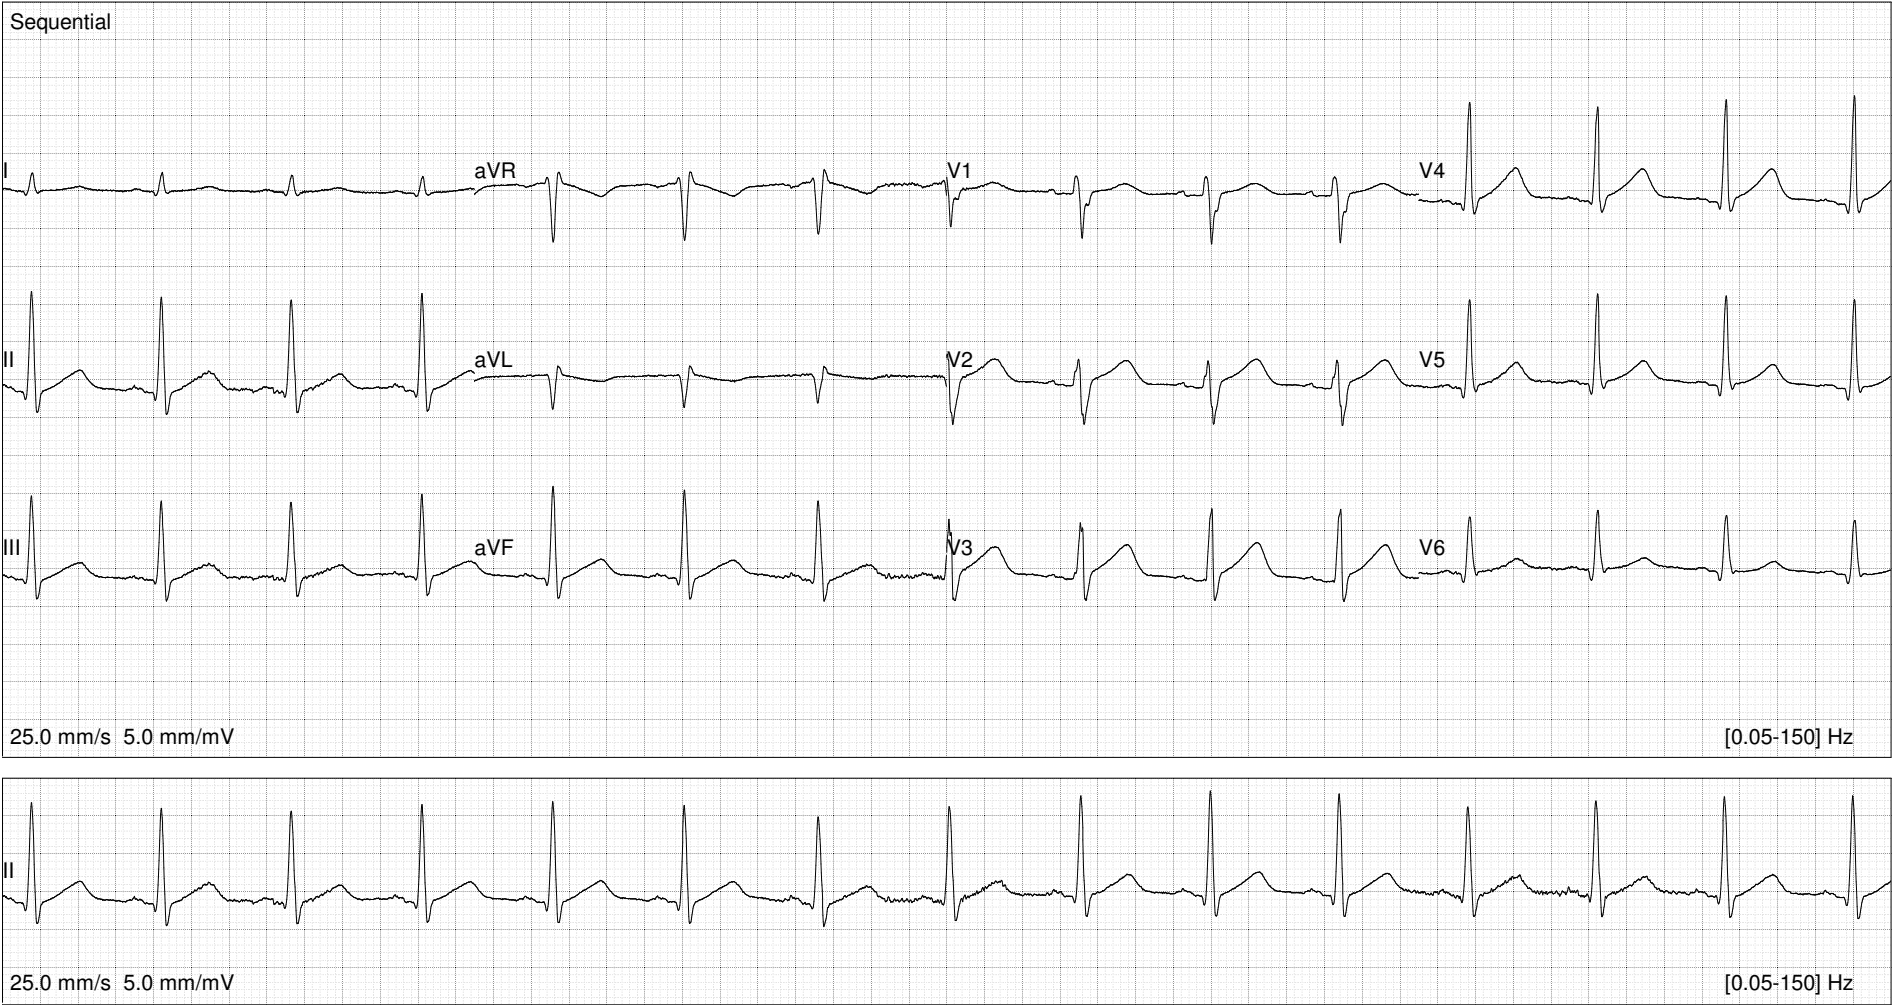



Anton Swart Biokinetic Rehabilitation Practice

Name: 004 004 004
Number: 004
Gender: Male
Birthdate: 13/11/1964 53 years
P / PQ: 113 ms / 143 ms
QRS: 109 ms
QT / QTc / QTd: 404 ms / 453 ms / -
P/QRS/T axis: 71° / 81° / 78°
Heartrate: 88 bpm

Recorded: 05/05/2018 12:18:48
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW



Beats		RR	
Total:	443	Minimum	630 ms
Normal:	443	Maximum	715 ms
Other:	0	Mean:	676 ms
		SD:	16 ms

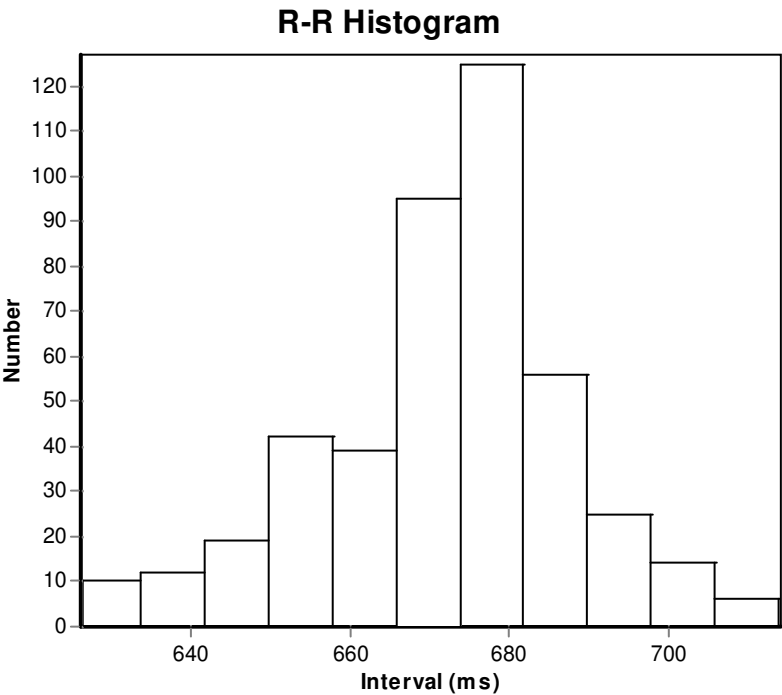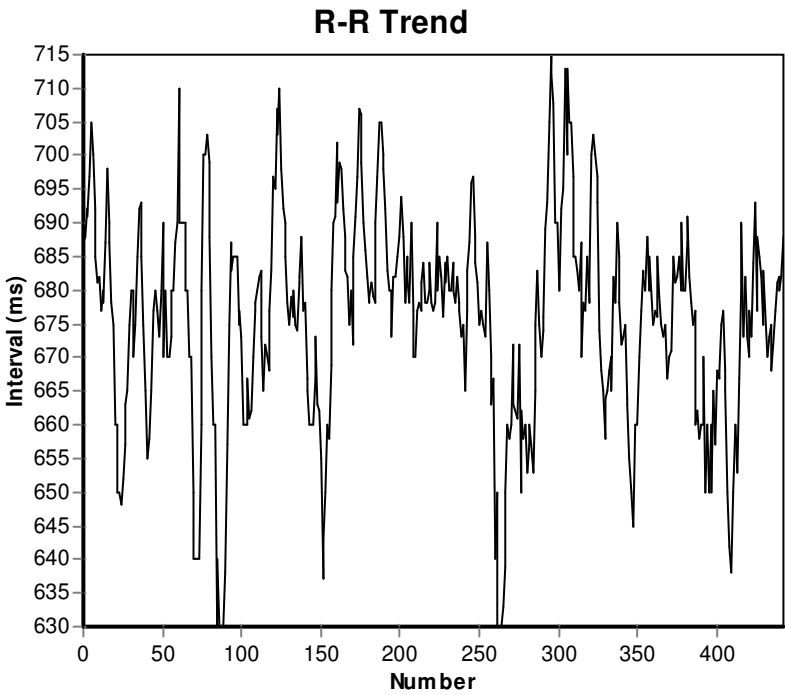

Heart Rate Variability: Time Domain Analysis

Name: 004, 004 004
Number: 004
Gender: Male


Birthdate: 13/11/1964
Recorded: 05/05/2018 12:18:48

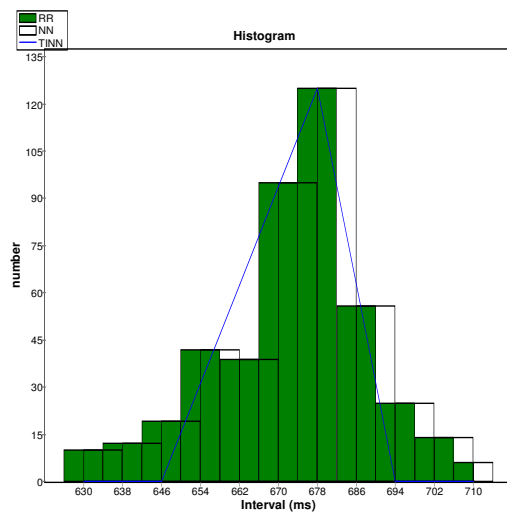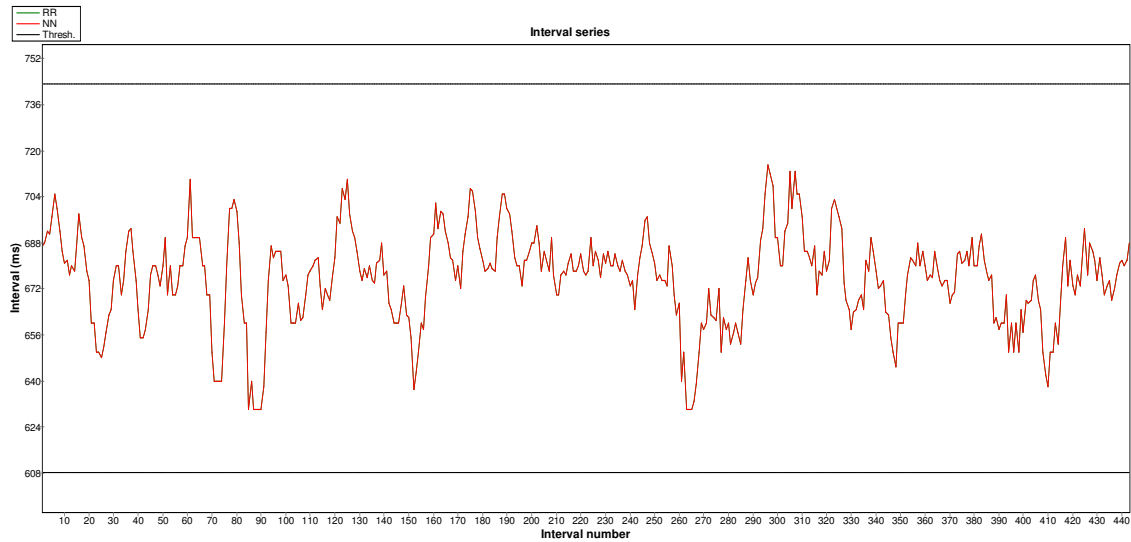

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	16	16
Triangular Interpolation (ms)	48	48
Triangular Index	3.54	3.54

Interval statistics	NN	RR
Number	443	443
Minimum (ms)	630	630
Maximum (ms)	715	715
Range (ms)	85	85
Avg (ms)	676	676
SD (ms)	16	16
AvgDev (ms)	12	12
p5 (ms)	648	648
p50 (ms)	678	678
p95 (ms)	700	700
Skewness	-0.50	-0.50
Kurtosis	3.56	3.56


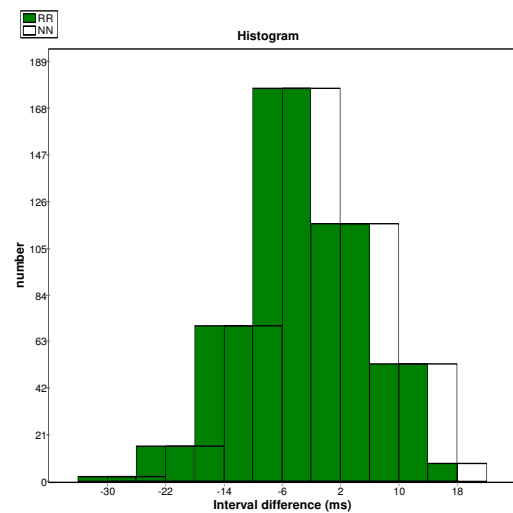


HRV parameters	NN	RR
SDSD (ms)	8	8
RMSSD (ms)	8	8
NN50	0	0
NN50(1)	0	0
NN50(2)	0	0
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	1.66	1.66
SD(Logarithmic Index)	0.25	0.25

Interval statistics	NN	RR
Number	442	442
Minimum (ms)	-30	-30
Maximum (ms)	20	20
Range (ms)	50	50
Avg (ms)	0	0
SD (ms)	8	8
AvgDev (ms)	6	6
p5 (ms)	-12	-12
p50 (ms)	0	0
p95 (ms)	12	12
Skewness	-0.20	-0.20
Kurtosis	3.46	3.46

Heart Rate Variability: Frequency Domain Analysis

Name: 004, 004 004 Birthdate: 13/11/1964
 Number: 004 Recorded: 05/05/2018 12:18:48
 Gender: Male

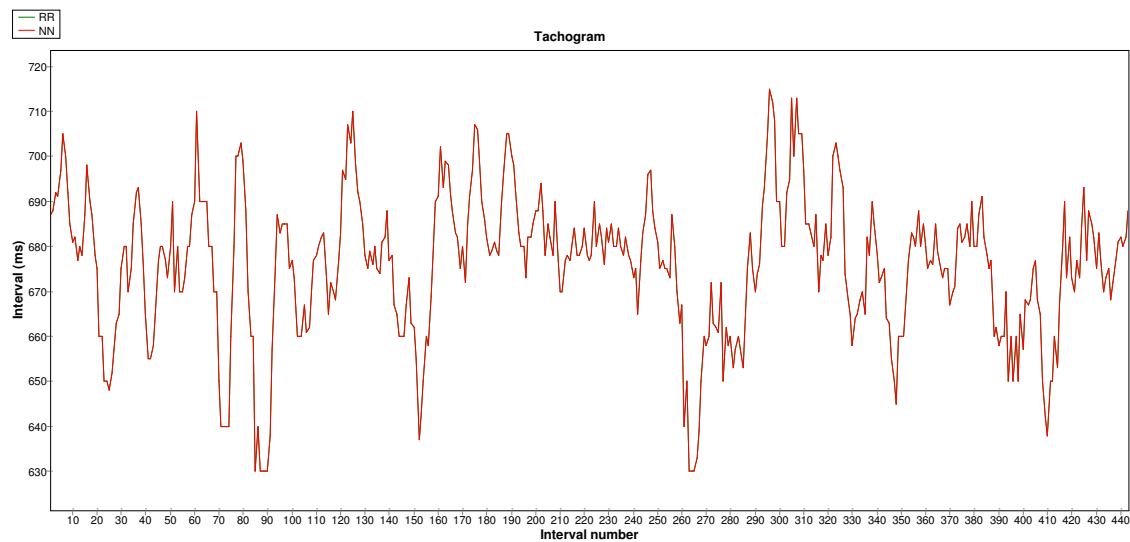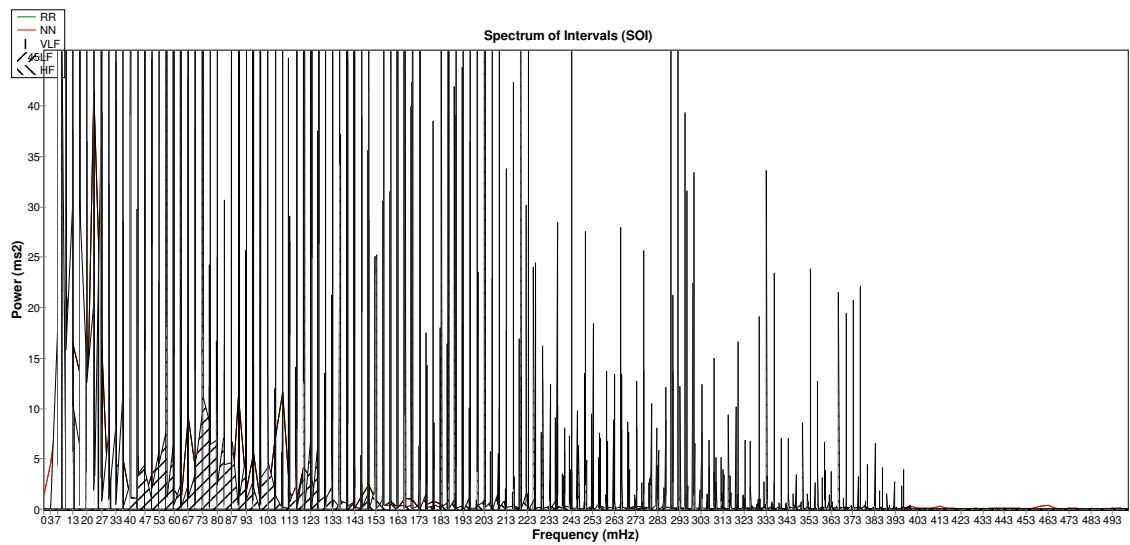

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	237	237	Spectrum of Intervals (SOI)	
VLF (ms2)	136	136	Frequency resolution (mHz)	3
LF (ms2)	89	89	VLF lower boundary (mHz)	3
HF (ms2)	12	12	VLF upper boundary (mHz)	40
LF/HF	7.53	7.53	LF upper boundary (mHz)	150
LF normalized	88.27	88.27	HF upper boundary (mHz)	400
HF normalized	11.73	11.73	Smoothing factor	1
VLF peak (mHz)	23	23	Tapering	Hann
LF peak (mHz)	110	110	Fourier transform	DFT
HF peak (mHz)	167	167	Sample frequency (Hz)	1.48
			Interval correction	Annotation
			Interval threshold (%)	10