


Anton Swart Biokinetic Rehabilitation Practice

Name: 006 006 006
Number: 006
Gender: Female
Birthdate: 25/01/1979 39 years

P / PQ: 108 ms / 175 ms
QRS: 92 ms
QT / QTc / QTd: 392 ms / 432 ms / -
P/QRS/T axis: 77° / 85° / 73°
Heartrate: 83 bpm

Recorded: 03/05/2018 18:08:27
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

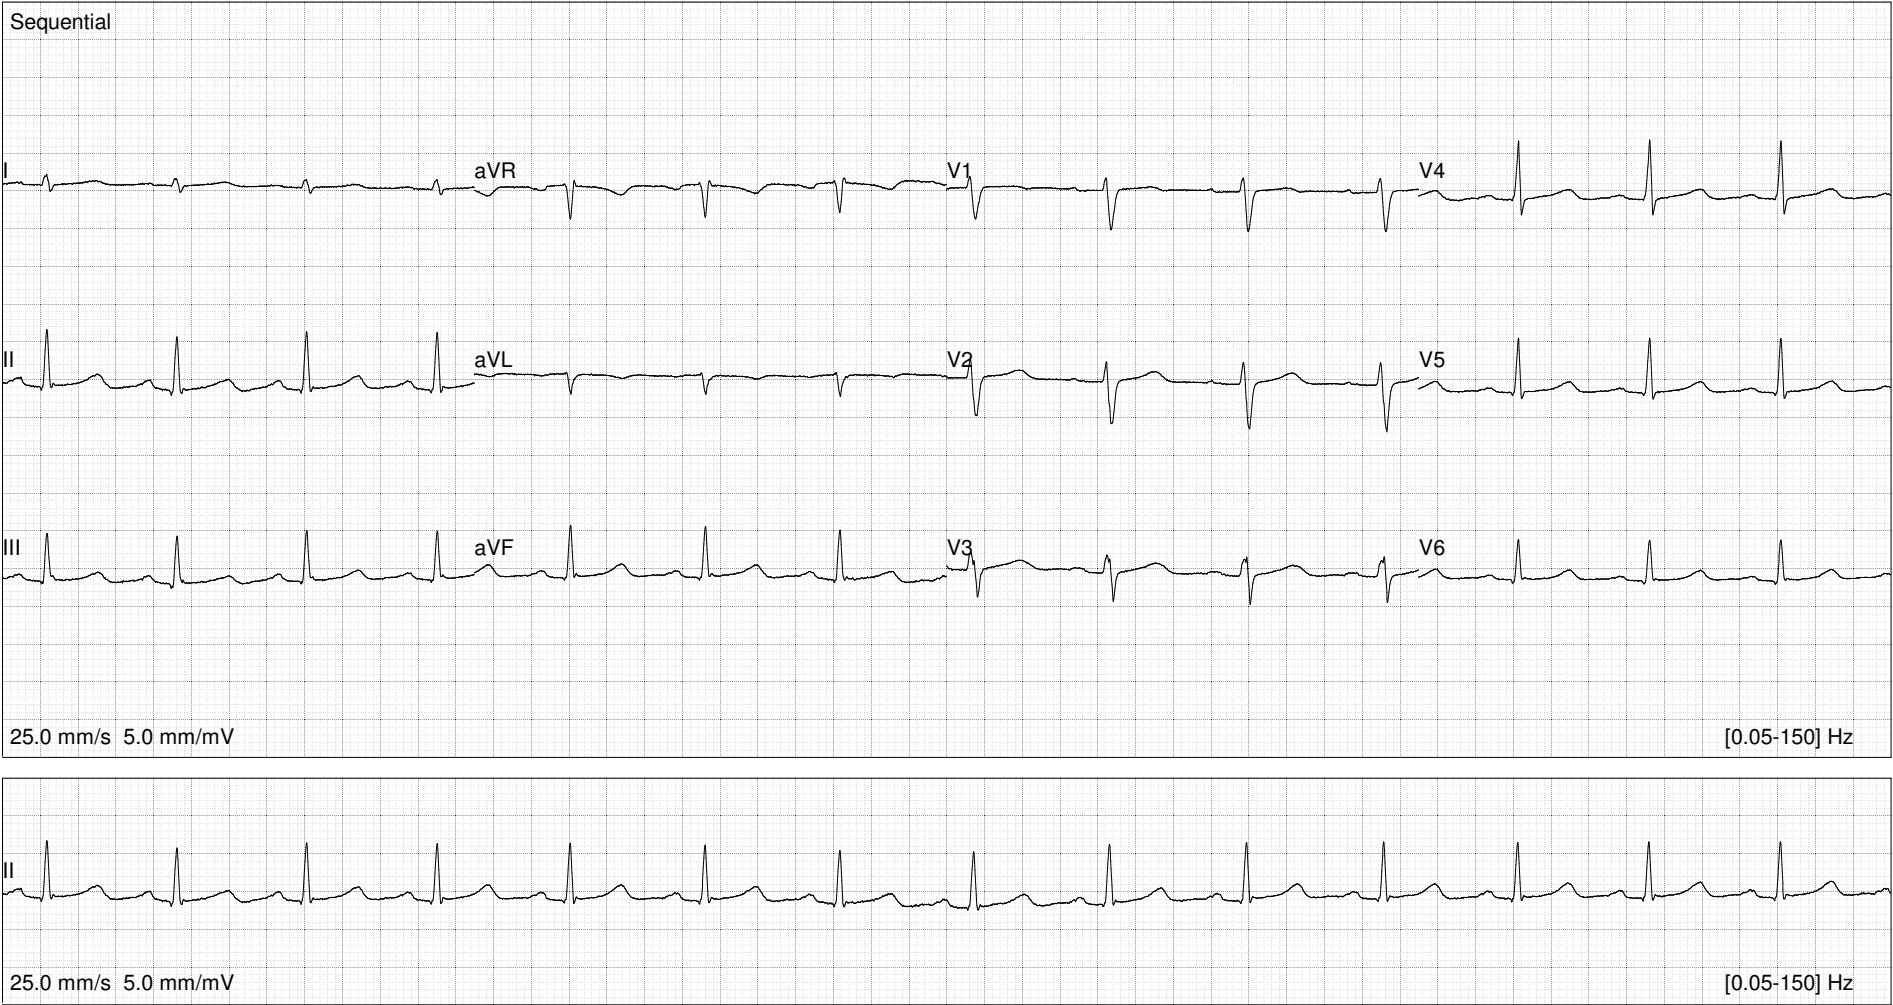

Anton Swart Biokinetic Rehabilitation Practice

Name:

006 006 006

Number:

006

Gender:

Female

Birthdate:

25/01/1979 39 years

P / PQ:

108 ms / 175 ms

QRS:

92 ms

QT / QTc / QTd:

392 ms / 432 ms / -

P/QRS/T axis:

77° / 85° / 73°

Heartrate:

83 bpm

Recorded:

03/05/2018 18:08:27

Recorded by:

Mr. Anton Swart

Referring physician:

Location:

Anton Swart Biokinetic Rehabilitation Practice



Ordering physician:

Attending physician:

Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW



Beats		RR	
Total:	415	Minimum	610 ms
Normal:	415	Maximum	860 ms
Other:	0	Mean:	722 ms
		SD:	29 ms

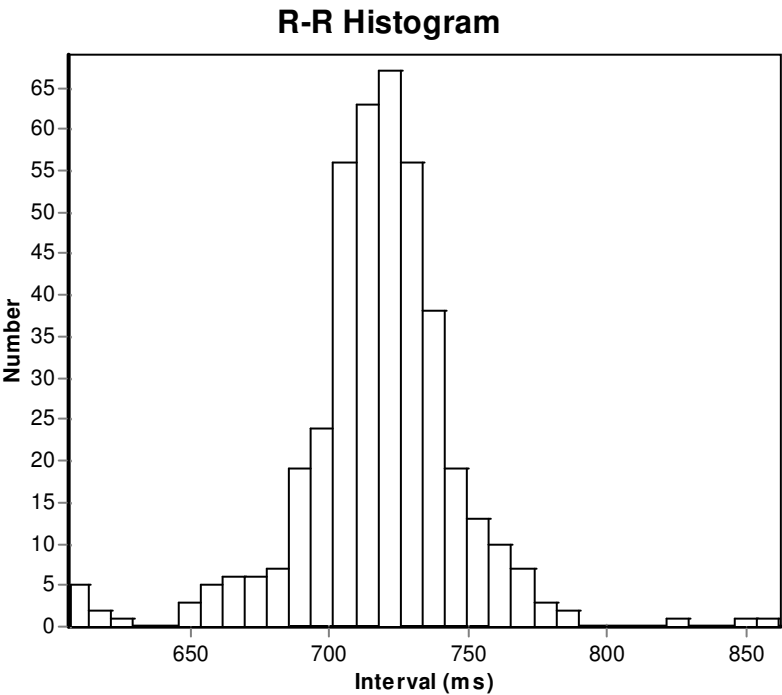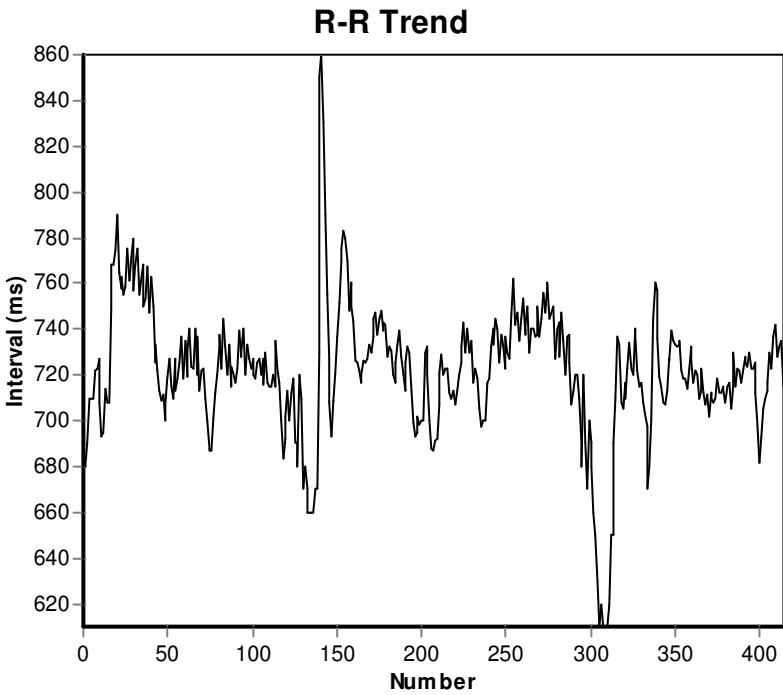

Heart Rate Variability: Time Domain Analysis

Name: 006, 006 006
 Number: 006
 Gender: Female


Birthdate: 25/01/1979
 Recorded: 03/05/2018 18:08:27

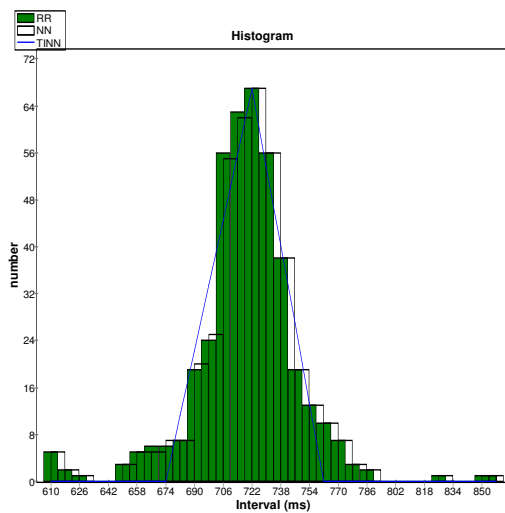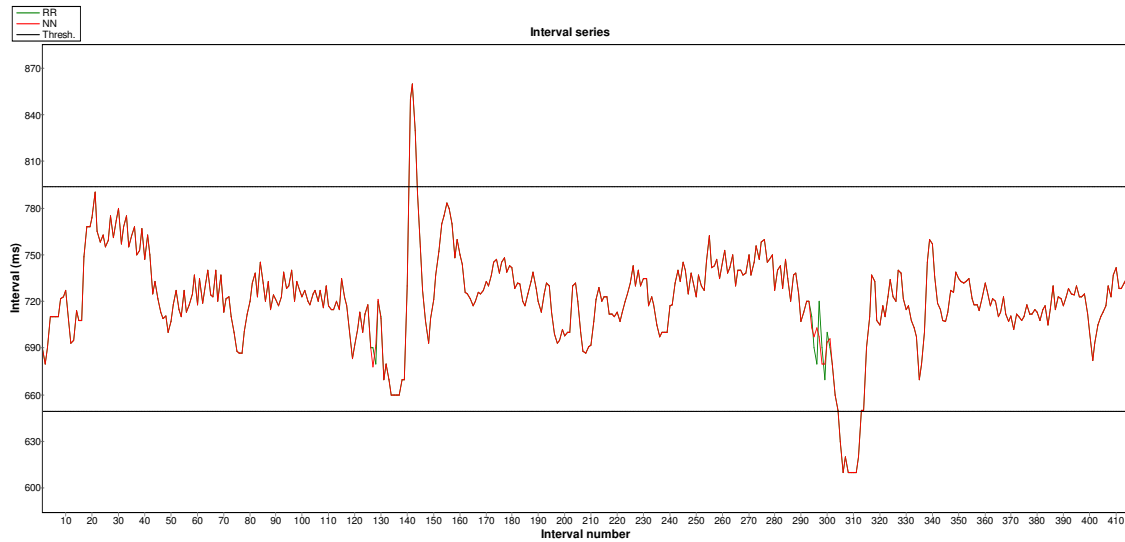

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	29	29
Triangular Interpolation (ms)	88	88
Triangular Index	6.19	6.19

Interval statistics	NN	RR
Number	415	415
Minimum (ms)	610	610
Maximum (ms)	860	860
Range (ms)	250	250
Avg (ms)	722	722
SD (ms)	29	29
AvgDev (ms)	20	20
p5 (ms)	670	670
p50 (ms)	723	723
p95 (ms)	767	767
Skewness	-0.37	-0.37
Kurtosis	7.51	7.48

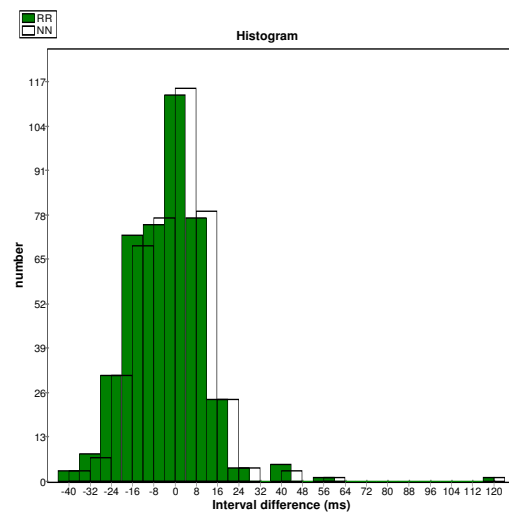



HRV parameters	NN	RR
SDSD (ms)	14	14
RMSSD (ms)	14	14
NN50	2	2
NN50(1)	0	0
NN50(2)	2	2
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	0.85	0.84
SD(Logarithmic Index)	0.10	0.15

Interval statistics	NN	RR
Number	414	414
Minimum (ms)	-40	-40
Maximum (ms)	120	120
Range (ms)	160	160
Avg (ms)	0	0
SD (ms)	14	14
AvgDev (ms)	10	10
p5 (ms)	-20	-20
p50 (ms)	0	0
p95 (ms)	18	19
Skewness	1.67	1.63
Kurtosis	16.57	15.39

Heart Rate Variability: Frequency Domain Analysis

Name: 006, 006 006
 Number: 006
 Gender: Female

Birthdate: 25/01/1979
 Recorded: 03/05/2018 18:08:27

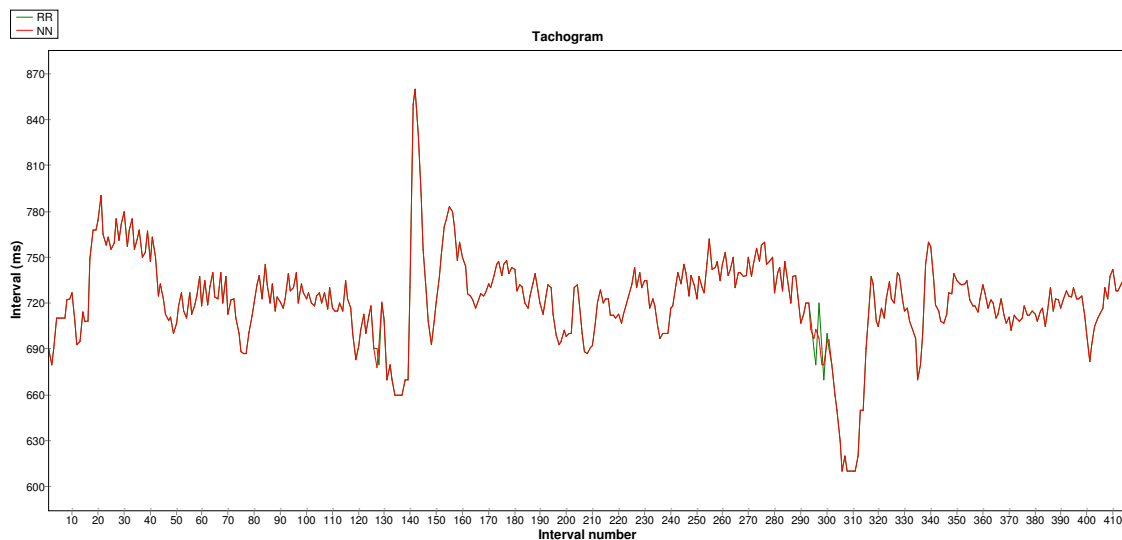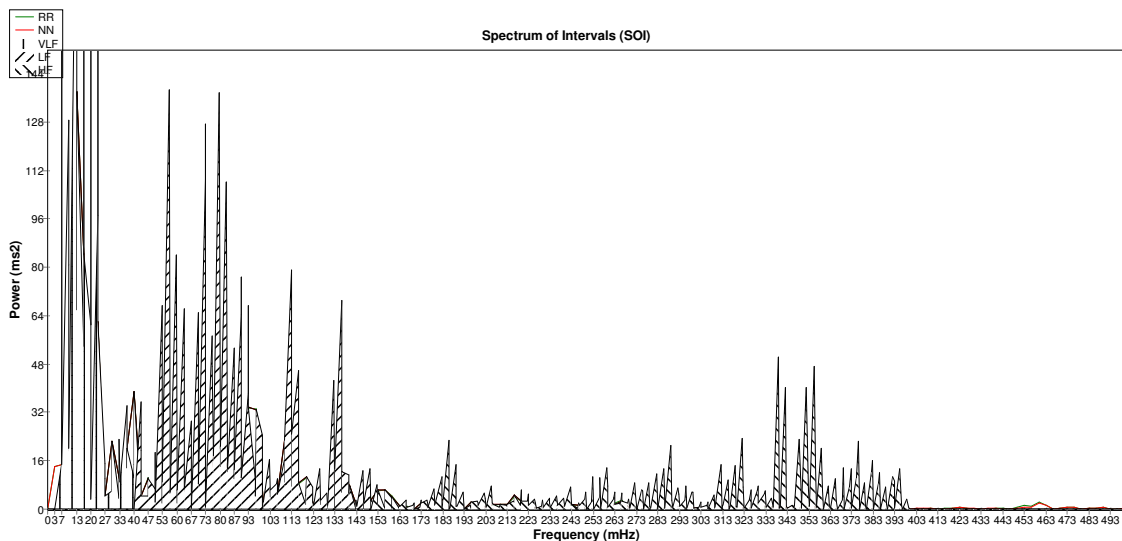

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	816	815	Spectrum of Intervals (SOI)	
VLF (ms2)	418	418	Frequency resolution (mHz)	3
LF (ms2)	323	323	VLF lower boundary (mHz)	3
HF (ms2)	75	74	VLF upper boundary (mHz)	40
LF/HF	4.31	4.34	LF upper boundary (mHz)	150
LF normalized	81.15	81.27	HF upper boundary (mHz)	400
HF normalized	18.85	18.73	Smoothing factor	1
VLF peak (mHz)	13	13	Tapering	Hann
LF peak (mHz)	93	93	Fourier transform	DFT
HF peak (mHz)	157	157	Sample frequency (Hz)	1.39
			Interval correction	Annotation
			Interval threshold (%)	10