


Anton Swart Biokinetic Rehabilitation Practice

Name: 007 007 007
Number: 007
Gender: Male
Birthdate: 25/12/1976 41 years

P / PQ: 110 ms / 148 ms
QRS: 100 ms
QT / QTc / QTd: 394 ms / 441 ms / -
P/QRS/T axis: 78° / 82° / 72°
Heartrate: 87 bpm

Recorded: 05/05/2018 11:57:14
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

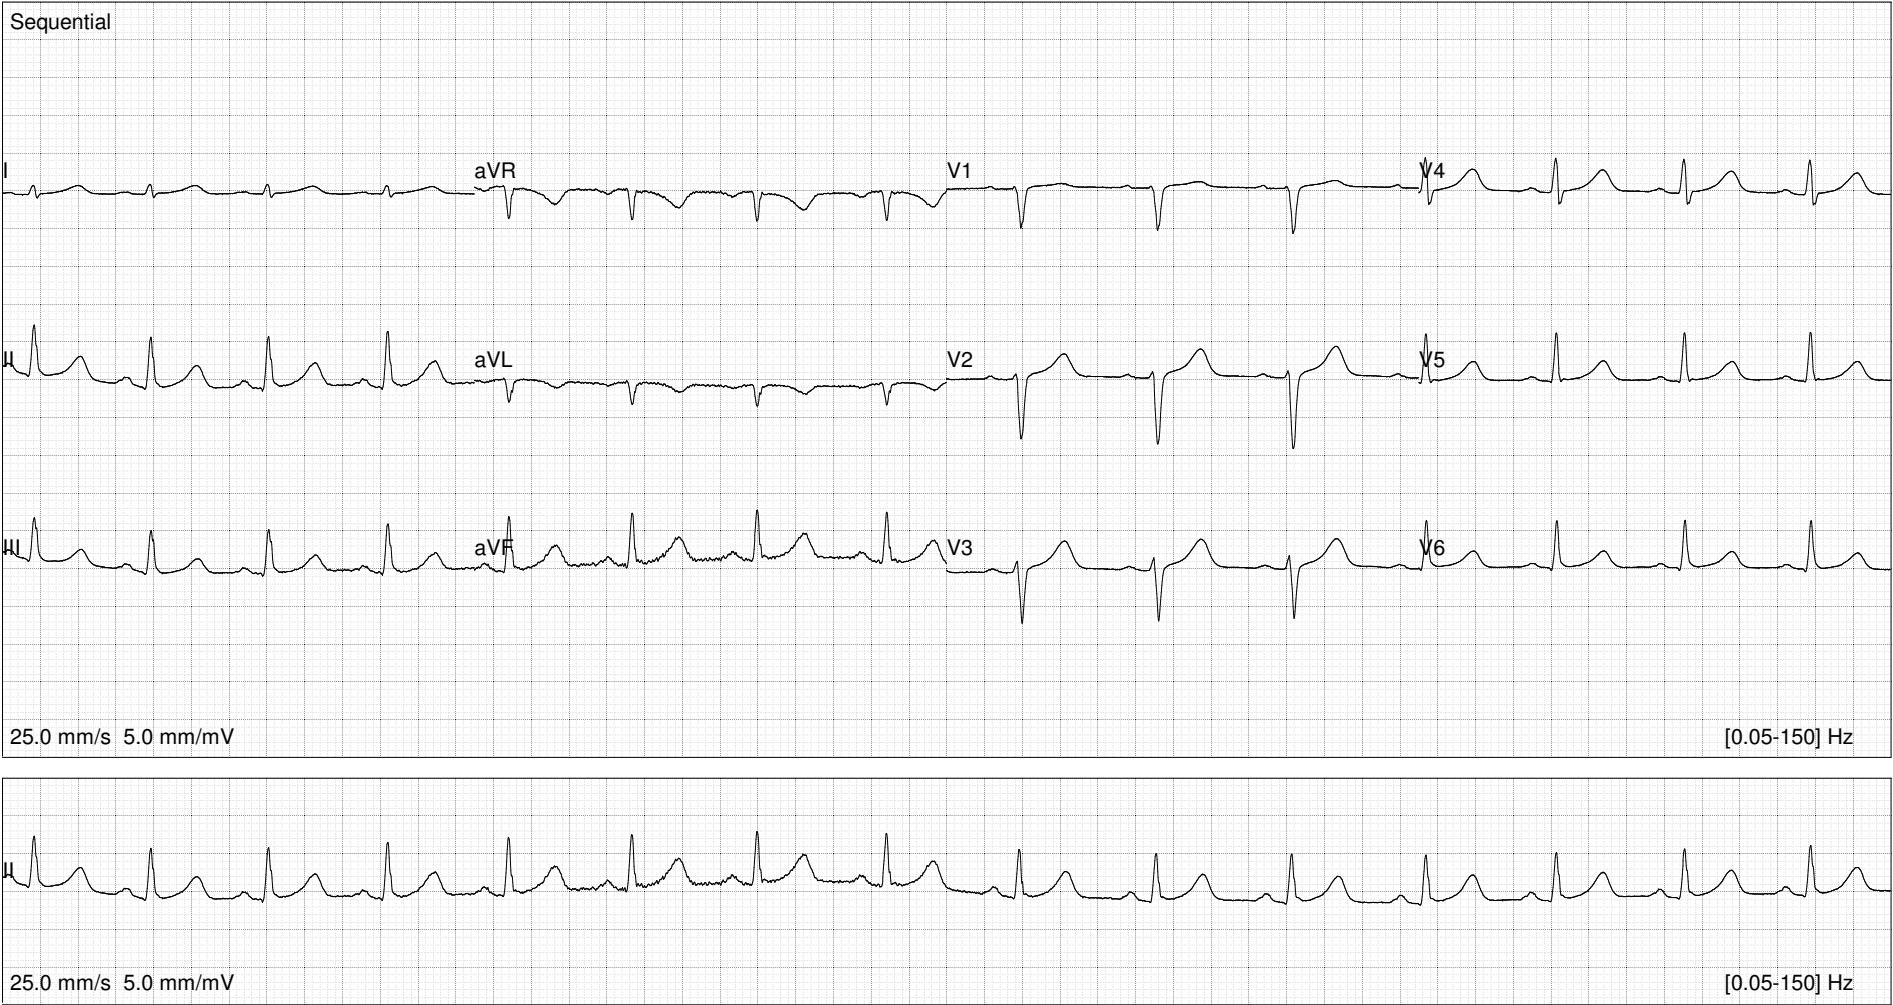



Anton Swart Biokinetic Rehabilitation Practice

Name: 007 007 007
Number: 007
Gender: Male
Birthdate: 25/12/1976 41 years
P / PQ: 110 ms / 148 ms
QRS: 100 ms
QT / QTc / QTd: 394 ms / 441 ms / -
P/QRS/T axis: 78° / 82° / 72°
Heartrate: 87 bpm

Recorded: 05/05/2018 11:57:14
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW



Beats		RR	
Total:	427	Minimum	460 ms
Normal:	427	Maximum	930 ms
Other:	0	Mean:	700 ms
		SD:	43 ms

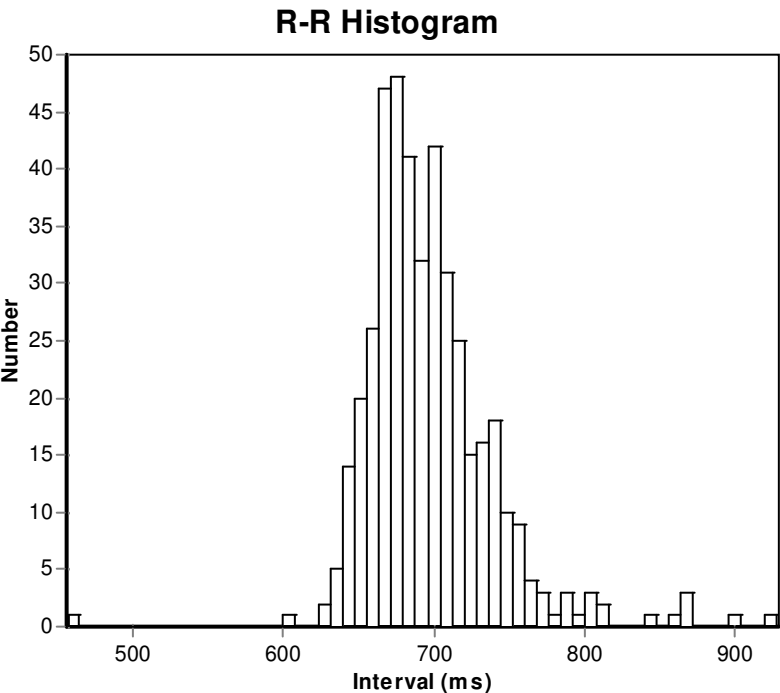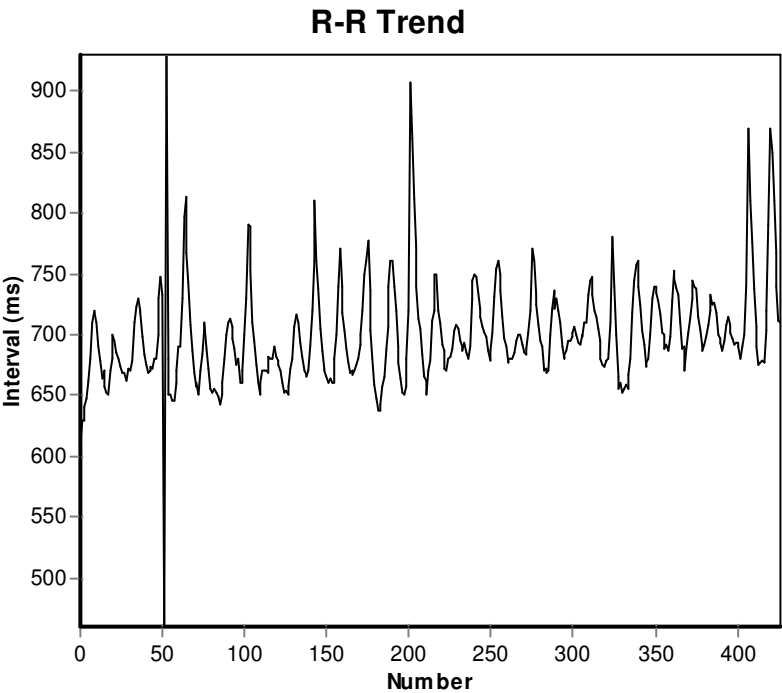

Heart Rate Variability: Time Domain Analysis

Name: 007, 007 007
Number: 007
Gender: Male


Birthdate: 25/12/1976
Recorded: 05/05/2018 11:57:14

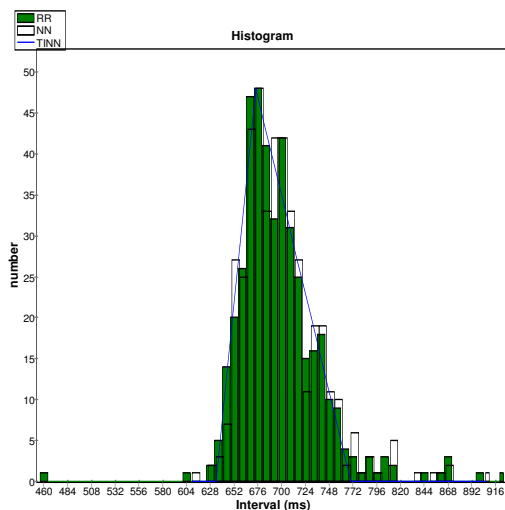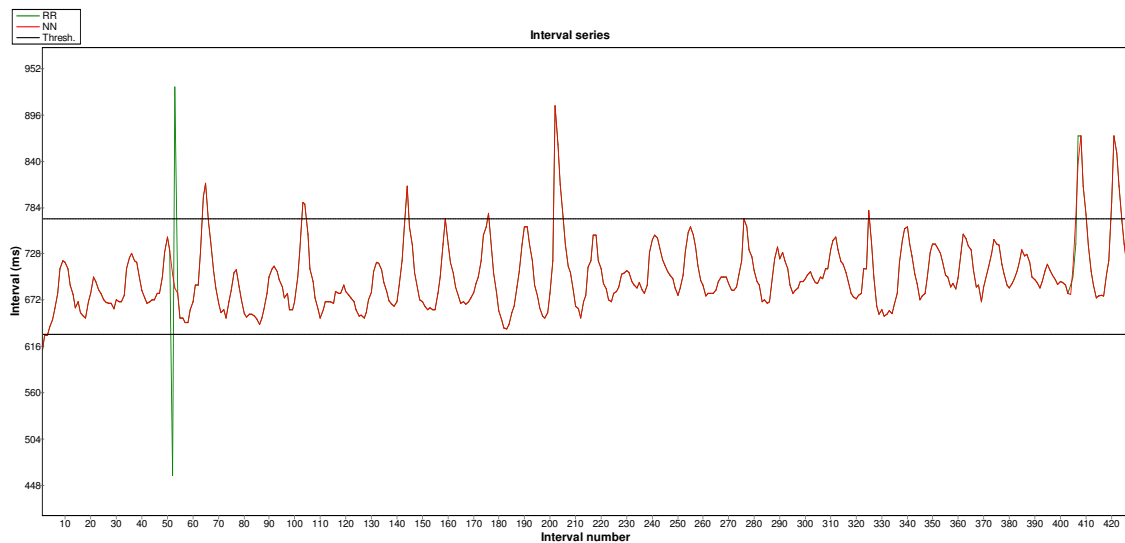

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	39	43
Triangular Interpolation (ms)	136	136
Triangular Index	8.90	8.90

Interval statistics	NN	RR
Number	427	427
Minimum (ms)	610	460
Maximum (ms)	907	930
Range (ms)	297	470
Avg (ms)	700	700
SD (ms)	39	43
AvgDev (ms)	29	30
p5 (ms)	651	650
p50 (ms)	693	693
p95 (ms)	770	770
Skewness	1.47	1.16
Kurtosis	6.86	9.61


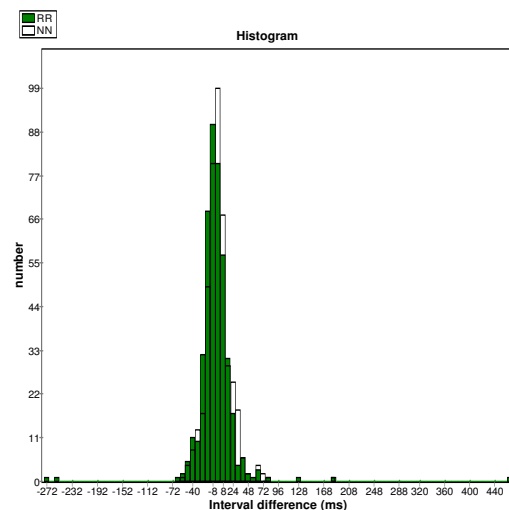


HRV parameters	NN	RR
SDSD (ms)	21	36
RMSSD (ms)	21	36
NN50	9	11
NN50(1)	1	3
NN50(2)	8	8
pNN50	0.02	0.03
pNN50(1)	0.00	0.01
pNN50(2)	0.02	0.02
Logarithmic Index	0.54	0.40
SD(Logarithmic Index)	0.03	0.04

Interval statistics	NN	RR
Number	426	426
Minimum (ms)	-60	-272
Maximum (ms)	187	470
Range (ms)	247	742
Avg (ms)	0	0
SD (ms)	21	36
AvgDev (ms)	14	16
p5 (ms)	-31	-33
p50 (ms)	-2	-2
p95 (ms)	31	30
Skewness	2.01	3.88
Kurtosis	17.77	82.94

Heart Rate Variability: Frequency Domain Analysis

Name: 007, 007 007 Birthdate: 25/12/1976
 Number: 007 Recorded: 05/05/2018 11:57:14
 Gender: Male

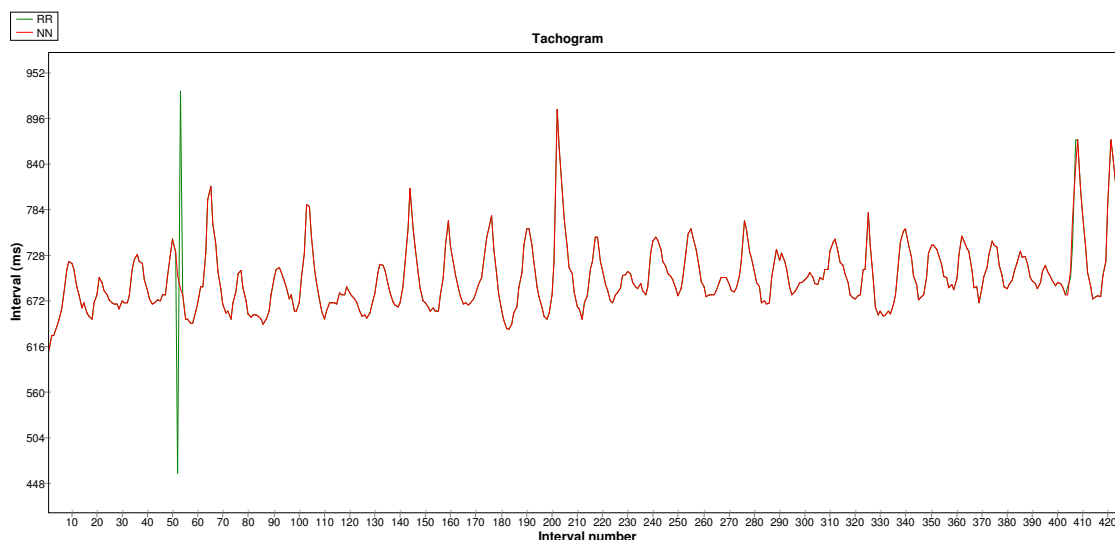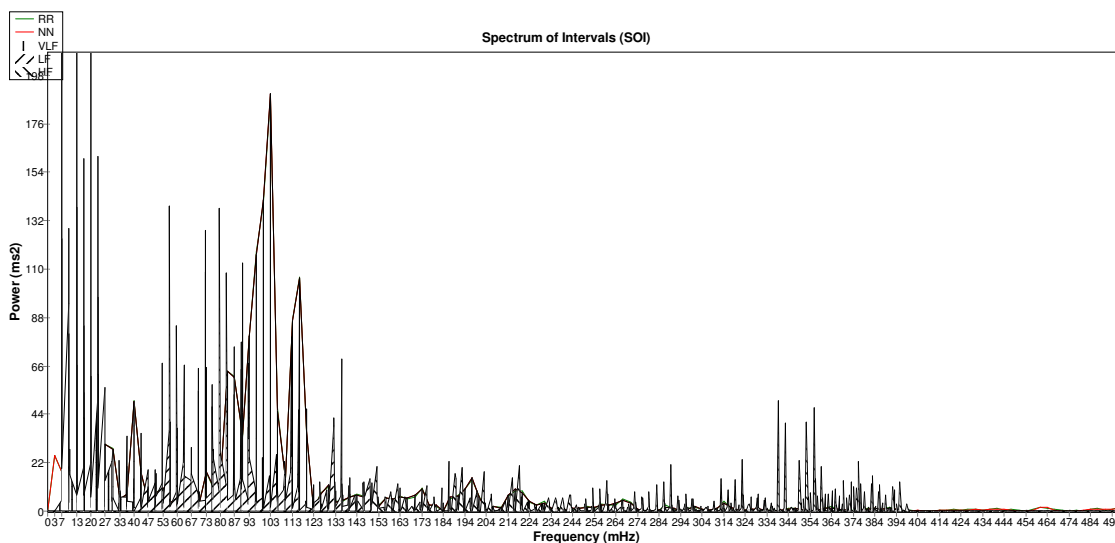

HRV parameters		NN	RR	HRV spectral settings	
TP (ms2)	1468	1471		Spectrum of Intervals (SOI)	
VLF (ms2)	151	152		Frequency resolution (mHz)	3
LF (ms2)	1121	1120		VLF lower boundary (mHz)	3
HF (ms2)	197	199		VLF upper boundary (mHz)	40
LF/HF	5.70	5.62		LF upper boundary (mHz)	150
LF normalized	85.07	84.89		HF upper boundary (mHz)	400
HF normalized	14.93	15.11		Smoothing factor	1
VLF peak (mHz)	40	40		Tapering	Hann
LF peak (mHz)	103	103		Fourier transform	DFT
HF peak (mHz)	197	197		Sample frequency (Hz)	1.43
				Interval correction	Annotation
				Interval threshold (%)	10