


Anton Swart Biokinetic Rehabilitation Practice

Name: 011 011 011
Number: 011
Gender: Male
Birthdate: 18/01/1976 42 years

Recorded: 03/05/2018 16:17:44
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

P / PQ: 122 ms / 187 ms
QRS: 83 ms
QT / QTc / QTd: 360 ms / 420 ms / -
P/QRS/T axis: 83° / 80° / 68°
Heartrate: 94 bpm

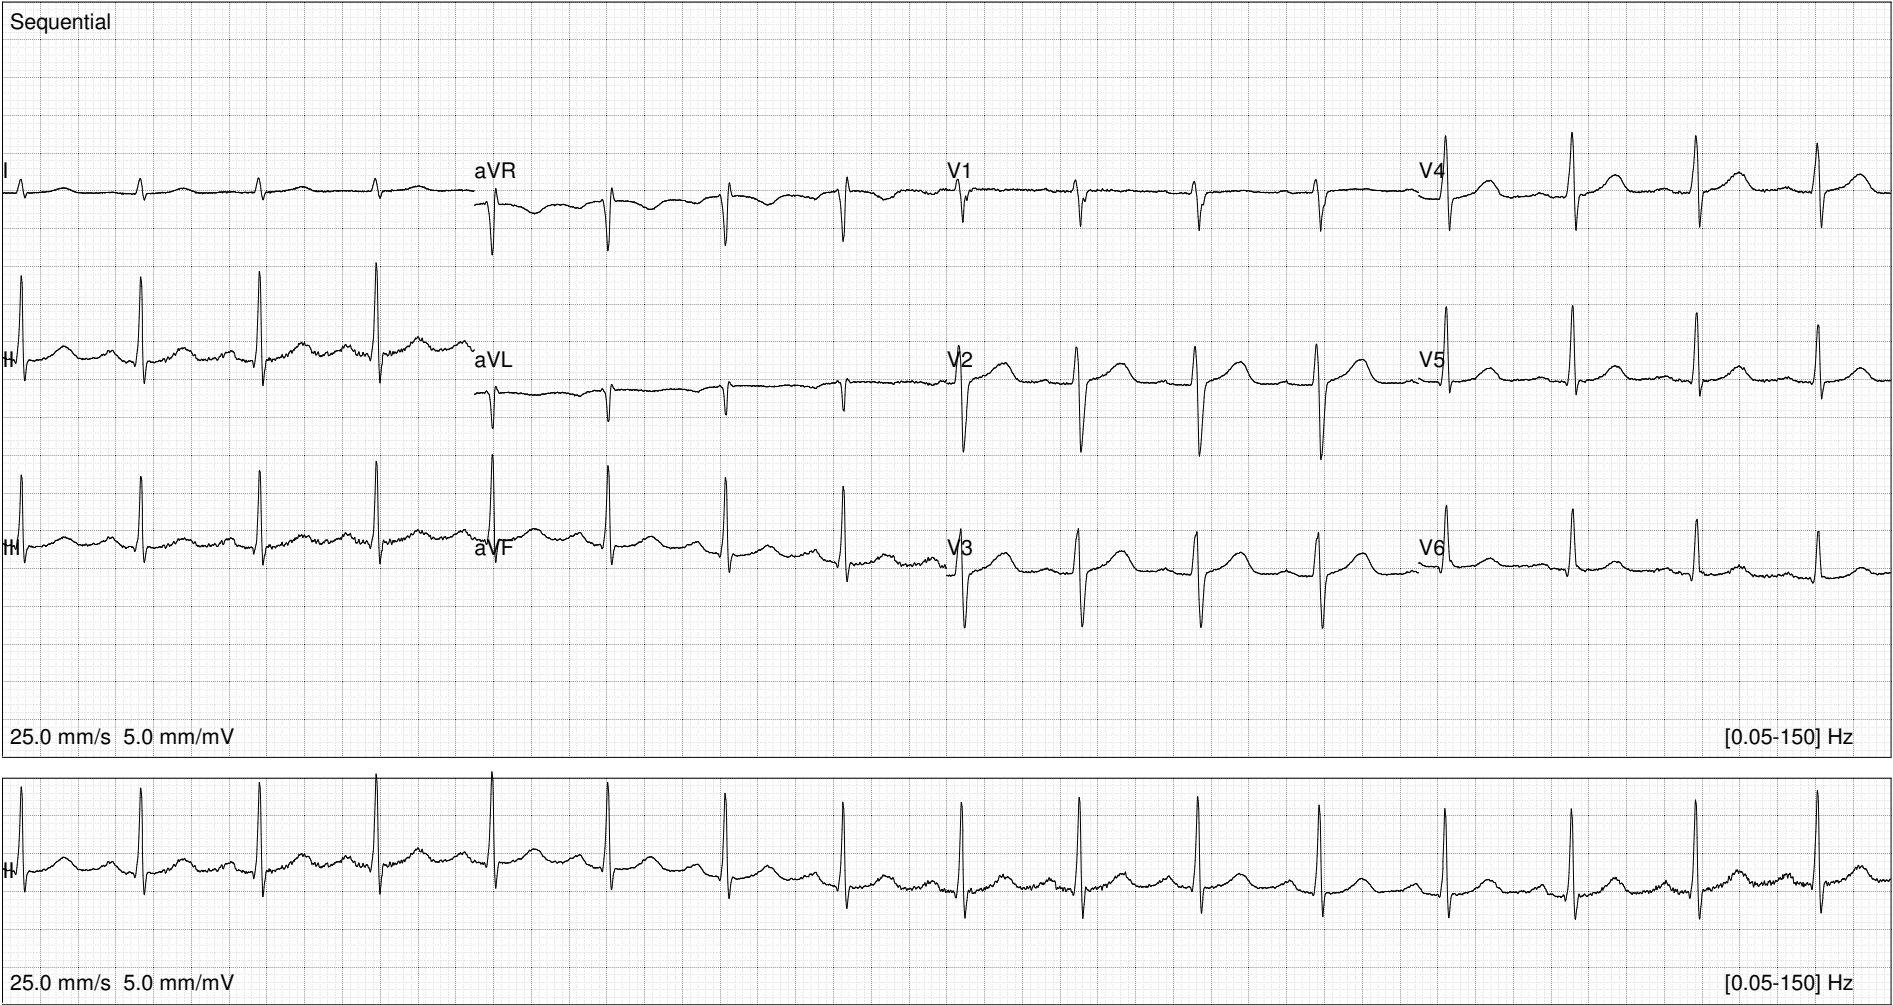

Anton Swart Biokinetic Rehabilitation Practice

Name: 011 011 011
Number: 011
Gender: Male
Birthdate: 18/01/1976 42 years


P / PQ: 122 ms / 187 ms
QRS: 83 ms
QT / QTc / QTd: 360 ms / 420 ms / -
P/QRS/T axis: 83° / 80° / 68°
Heartrate: 94 bpm

Recorded: 03/05/2018 16:17:44
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:


UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	464	Minimum	600 ms
Normal:	464	Maximum	746 ms
Other:	0	Mean:	645 ms
		SD:	23 ms

R-R Trend

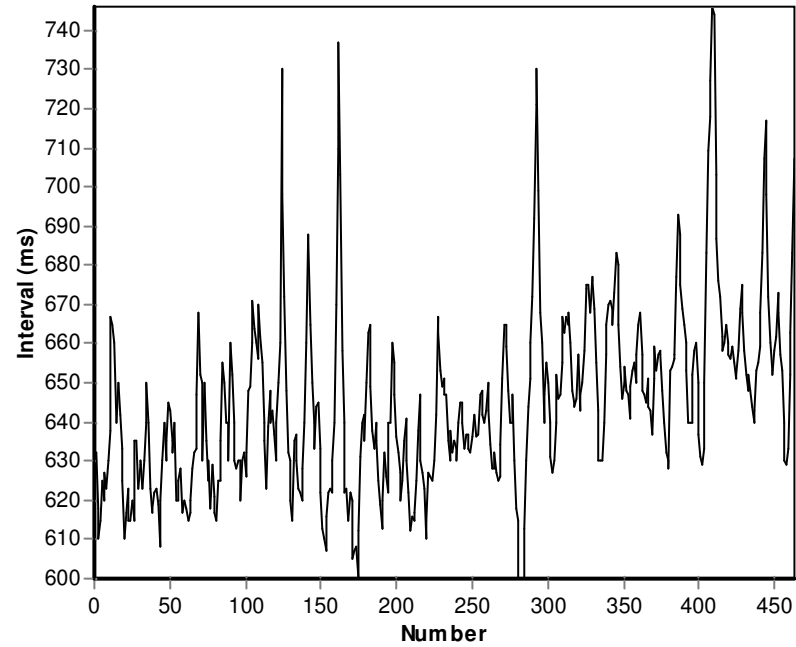



R-R Histogram

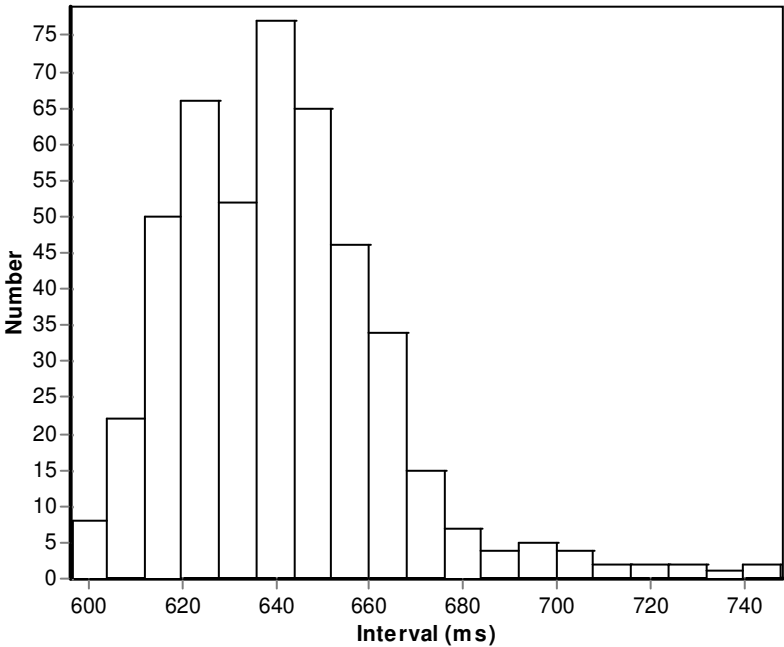

Heart Rate Variability: Time Domain Analysis

Name: 011, 011 011
 Number: 011
 Gender: Male


Birthdate: 18/01/1976
 Recorded: 03/05/2018 16:17:44

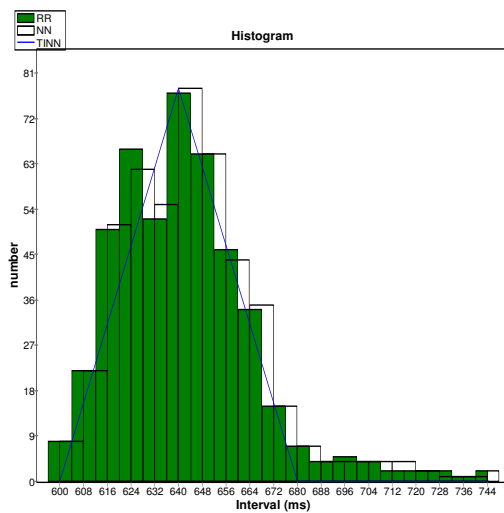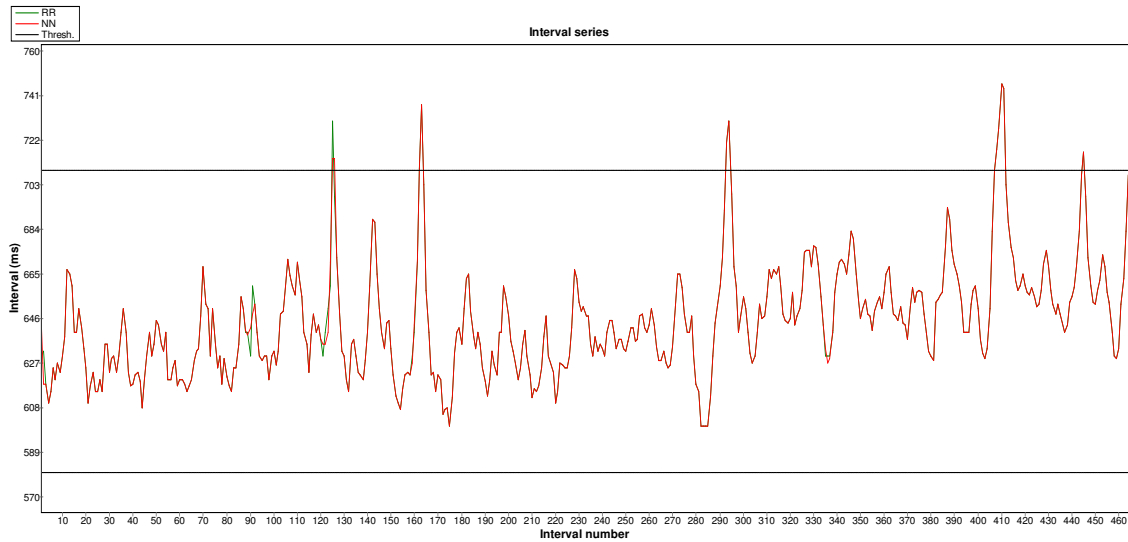

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	23	23
Triangular Interpolation (ms)	80	80
Triangular Index	5.95	6.03

Interval statistics	NN	RR
Number	464	464
Minimum (ms)	600	600
Maximum (ms)	746	746
Range (ms)	146	146
Avg (ms)	645	645
SD (ms)	23	23
AvgDev (ms)	18	18
p5 (ms)	615	615
p50 (ms)	641	640
p95 (ms)	687	687
Skewness	1.18	1.20
Kurtosis	5.48	5.58


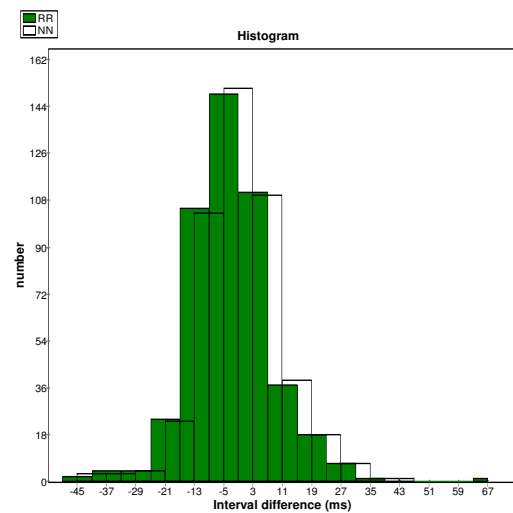


HRV parameters	NN	RR
SDSD (ms)	11	11
RMSSD (ms)	11	11
NN50	0	1
NN50(1)	0	0
NN50(2)	0	1
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	0.95	0.96
SD(Logarithmic Index)	0.11	0.07

Interval statistics	NN	RR
Number	463	463
Minimum (ms)	-45	-45
Maximum (ms)	44	70
Range (ms)	89	115
Avg (ms)	0	0
SD (ms)	11	11
AvgDev (ms)	8	8
p5 (ms)	-16	-16
p50 (ms)	0	0
p95 (ms)	20	20
Skewness	0.04	0.47
Kurtosis	4.88	6.81

Heart Rate Variability: Frequency Domain Analysis

Name: 011, 011 011 Birthdate: 18/01/1976
 Number: 011 Recorded: 03/05/2018 16:17:44
 Gender: Male

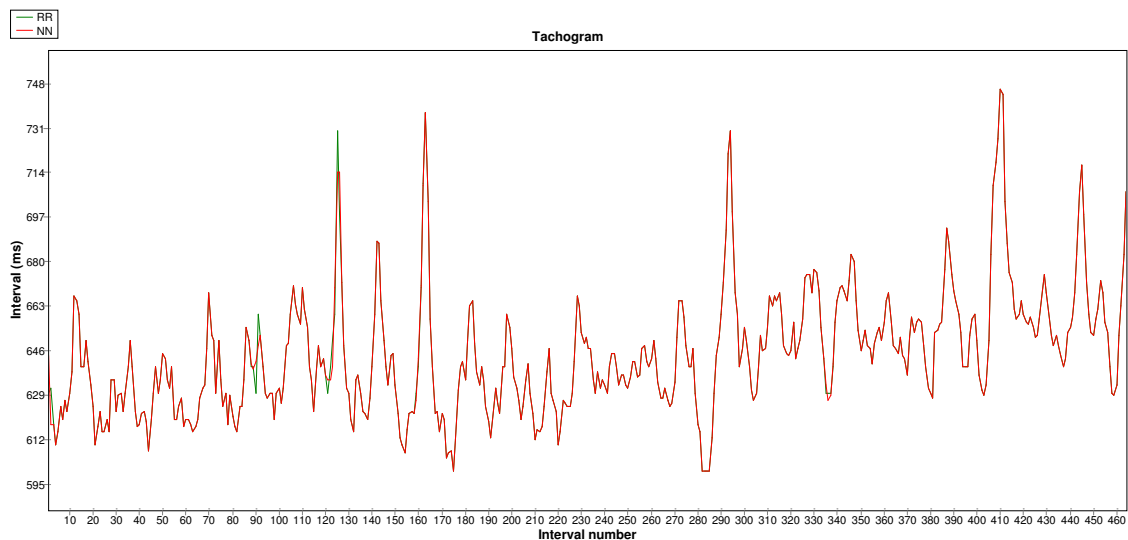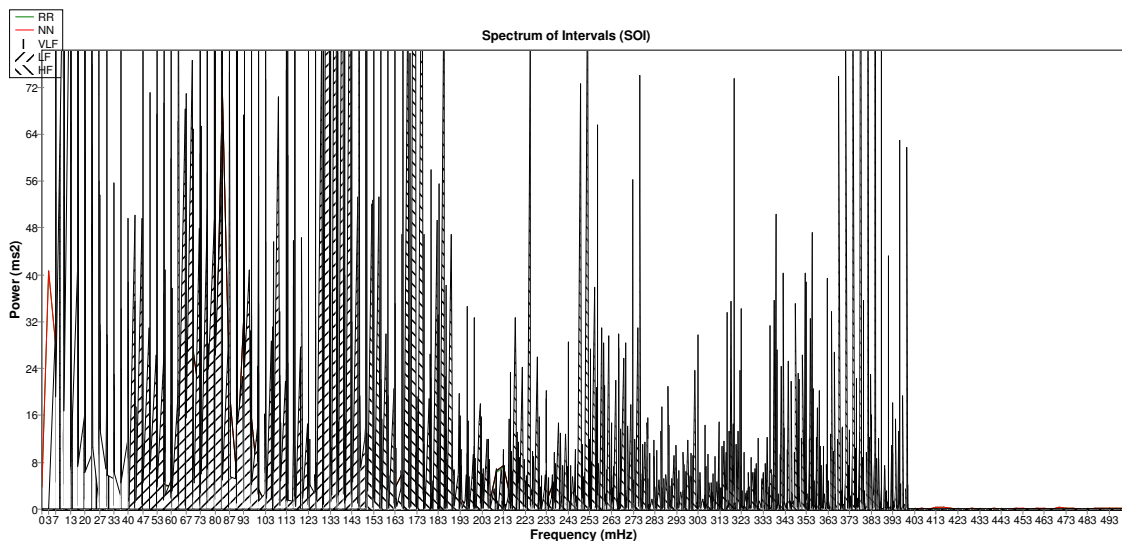

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	425	424	Spectrum of Intervals (SOI)	
VLF (ms2)	54	55	Frequency resolution (mHz)	3
LF (ms2)	292	291	VLF lower boundary (mHz)	3
HF (ms2)	79	78	VLF upper boundary (mHz)	40
LF/HF	3.69	3.72	LF upper boundary (mHz)	150
LF normalized	78.70	78.82	HF upper boundary (mHz)	400
HF normalized	21.30	21.18	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	83	83	Fourier transform	DFT
HF peak (mHz)	213	213	Sample frequency (Hz)	1.55
			Interval correction	Annotation
			Interval threshold (%)	10