


Anton Swart Biokinetic Rehabilitation Practice

Name: 014 014 014
Number: 014
Gender: Male
Birthdate: 13/06/1972 45 years

P / PQ: 82 ms / 157 ms
QRS: 93 ms
QT / QTc / QTd: 410 ms / 412 ms / -
P/QRS/T axis: 29° / 80° / 64°
Heartrate: 61 bpm

Recorded: 01/05/2018 16:46:57
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

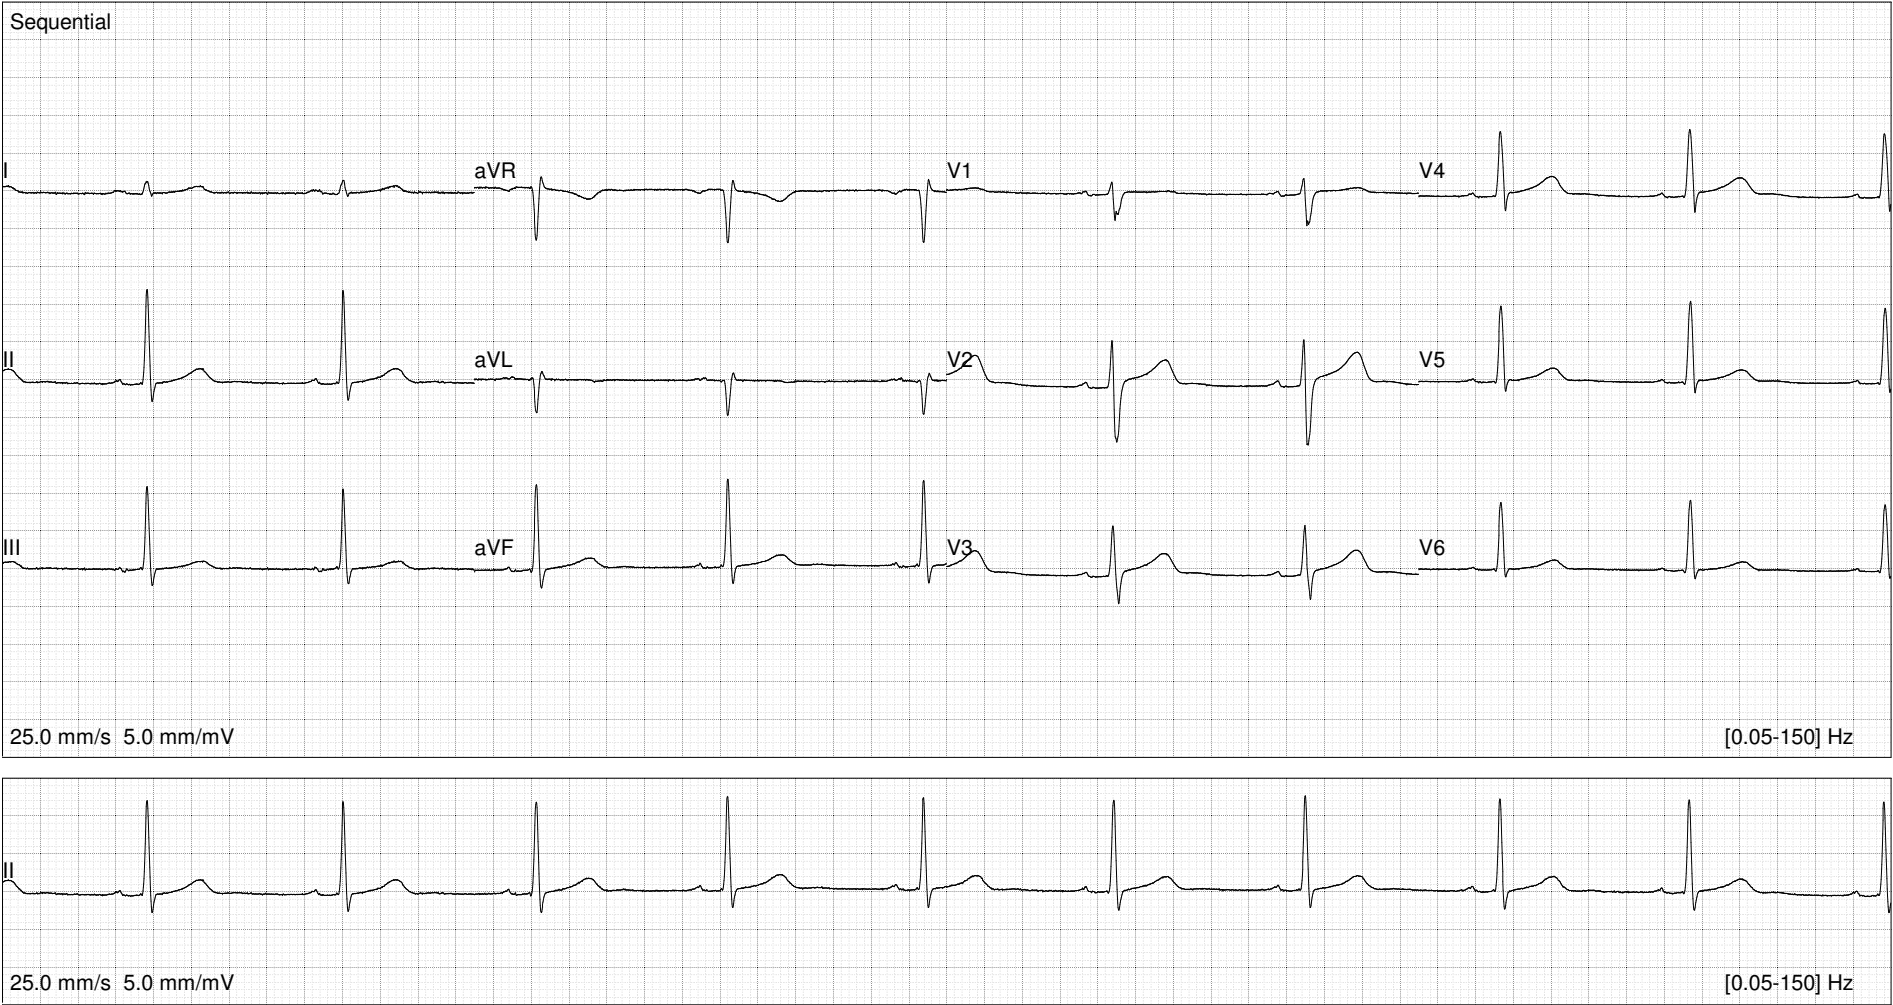

Anton Swart Biokinetic Rehabilitation Practice



Name: 014 014 014
Number: 014
Gender: Male
Birthdate: 13/06/1972 45 years

P / PQ: 82 ms / 157 ms
QRS: 93 ms
QT / QTc / QTd: 410 ms / 412 ms / -
P/QRS/T axis: 29° / 80° / 64°
Heartrate: 61 bpm

Recorded: 01/05/2018 16:46:57
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW



Beats		RR	
Total:	305	Minimum	911 ms
Normal:	305	Maximum	1050 ms
Other:	0	Mean:	980 ms
		SD:	28 ms

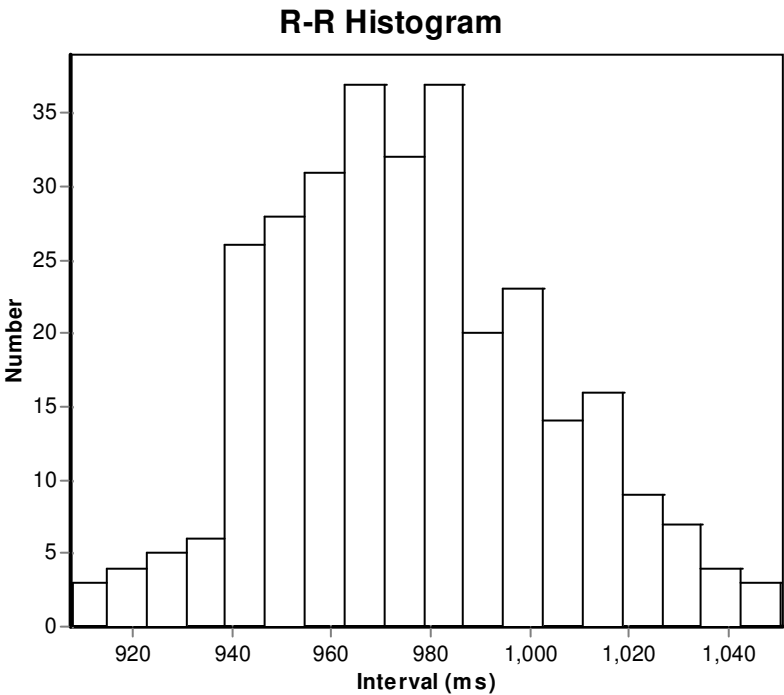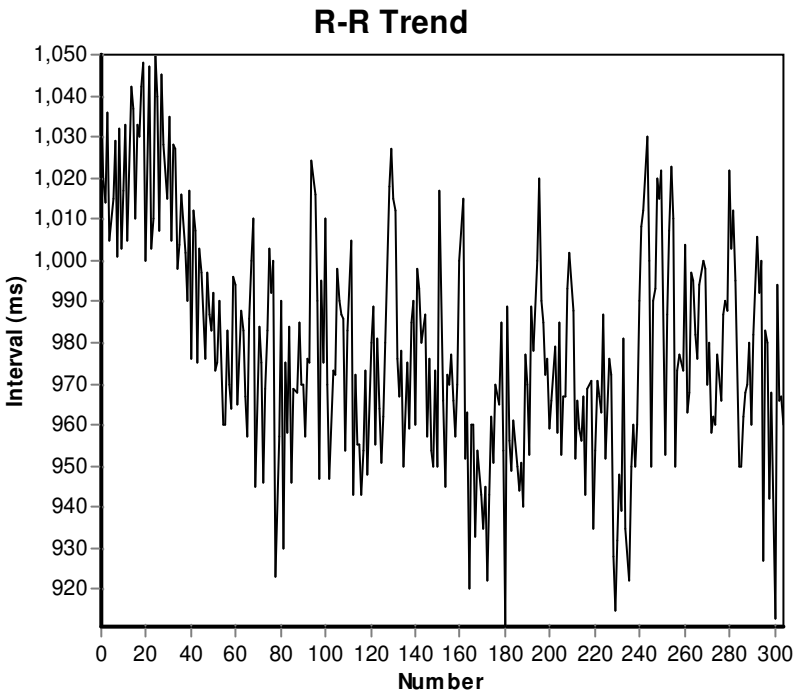

Heart Rate Variability: Time Domain Analysis

Name: 014, 014 014
Number: 014
Gender: Male


Birthdate: 13/06/1972
Recorded: 01/05/2018 16:46:57

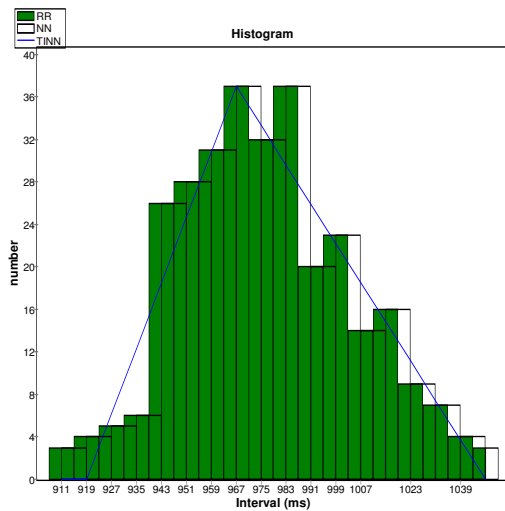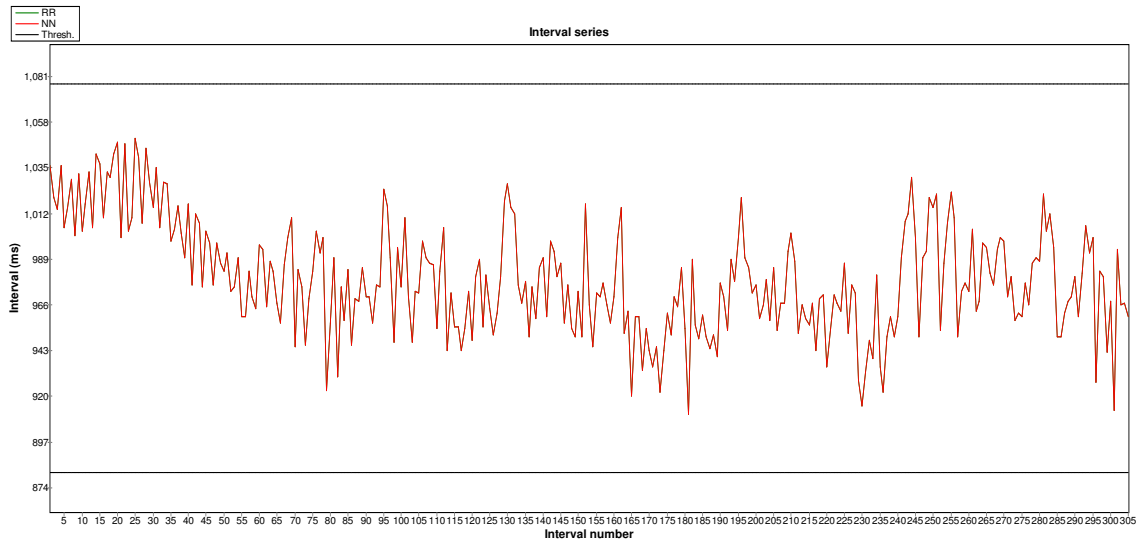

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	28	28
Triangular Interpolation (ms)	128	128
Triangular Index	8.24	8.24

Interval statistics	NN	RR
Number	305	305
Minimum (ms)	911	911
Maximum (ms)	1050	1050
Range (ms)	139	139
Avg (ms)	980	980
SD (ms)	28	28
AvgDev (ms)	23	23
p5 (ms)	939	939
p50 (ms)	976	976
p95 (ms)	1030	1030
Skewness	0.24	0.24
Kurtosis	2.73	2.73


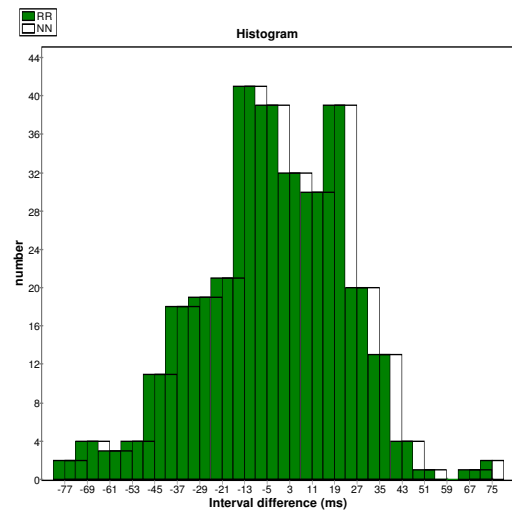


HRV parameters	NN	RR
SDSD (ms)	26	26
RMSSD (ms)	26	26
NN50	14	14
NN50(1)	10	10
NN50(2)	4	4
pNN50	0.05	0.05
pNN50(1)	0.03	0.03
pNN50(2)	0.01	0.01
Logarithmic Index	0.44	0.44
SD(Logarithmic Index)	0.03	0.03

Interval statistics	NN	RR
Number	304	304
Minimum (ms)	-77	-77
Maximum (ms)	81	81
Range (ms)	158	158
Avg (ms)	-0	-0
SD (ms)	26	26
AvgDev (ms)	21	21
p5 (ms)	-44	-44
p50 (ms)	-1	-1
p95 (ms)	38	38
Skewness	-0.20	-0.20
Kurtosis	3.23	3.23

Heart Rate Variability: Frequency Domain Analysis

Name: 014, 014 014 Birthdate: 13/06/1972
 Number: 014 Recorded: 01/05/2018 16:46:57
 Gender: Male

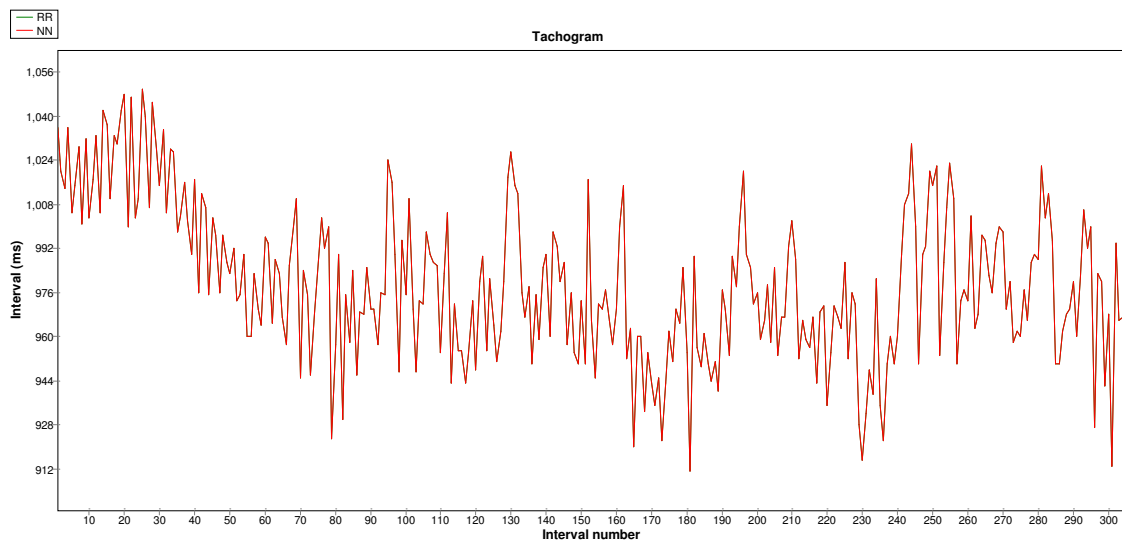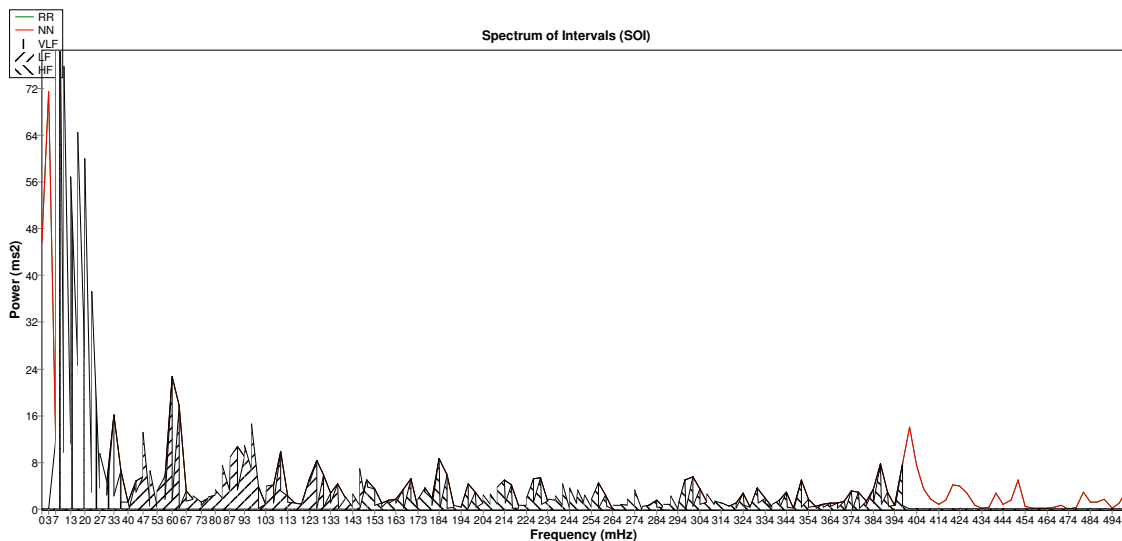

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	436	436	Spectrum of Intervals (SOI)	
VLF (ms2)	118	118	Frequency resolution (mHz)	3
LF (ms2)	152	152	VLF lower boundary (mHz)	3
HF (ms2)	166	166	VLF upper boundary (mHz)	40
LF/HF	0.92	0.92	LF upper boundary (mHz)	150
LF normalized	47.83	47.83	HF upper boundary (mHz)	400
HF normalized	52.17	52.17	Smoothing factor	1
VLF peak (mHz)	20	20	Tapering	Hann
LF peak (mHz)	60	60	Fourier transform	DFT
HF peak (mHz)	184	184	Sample frequency (Hz)	1.02
			Interval correction	Annotation
			Interval threshold (%)	10