


Anton Swart Biokinetic Rehabilitation Practice

Name: 014 014 014
Number: 014
Gender: Male
Birthdate: 13/06/1972 45 years

Recorded: 03/05/2018 17:07:49
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

P / PQ: 112 ms / 173 ms
QRS: 87 ms
QT / QTc / QTd: 359 ms / 415 ms / -
P/QRS/T axis: 76° / 78° / 50°
Heartrate: 92 bpm

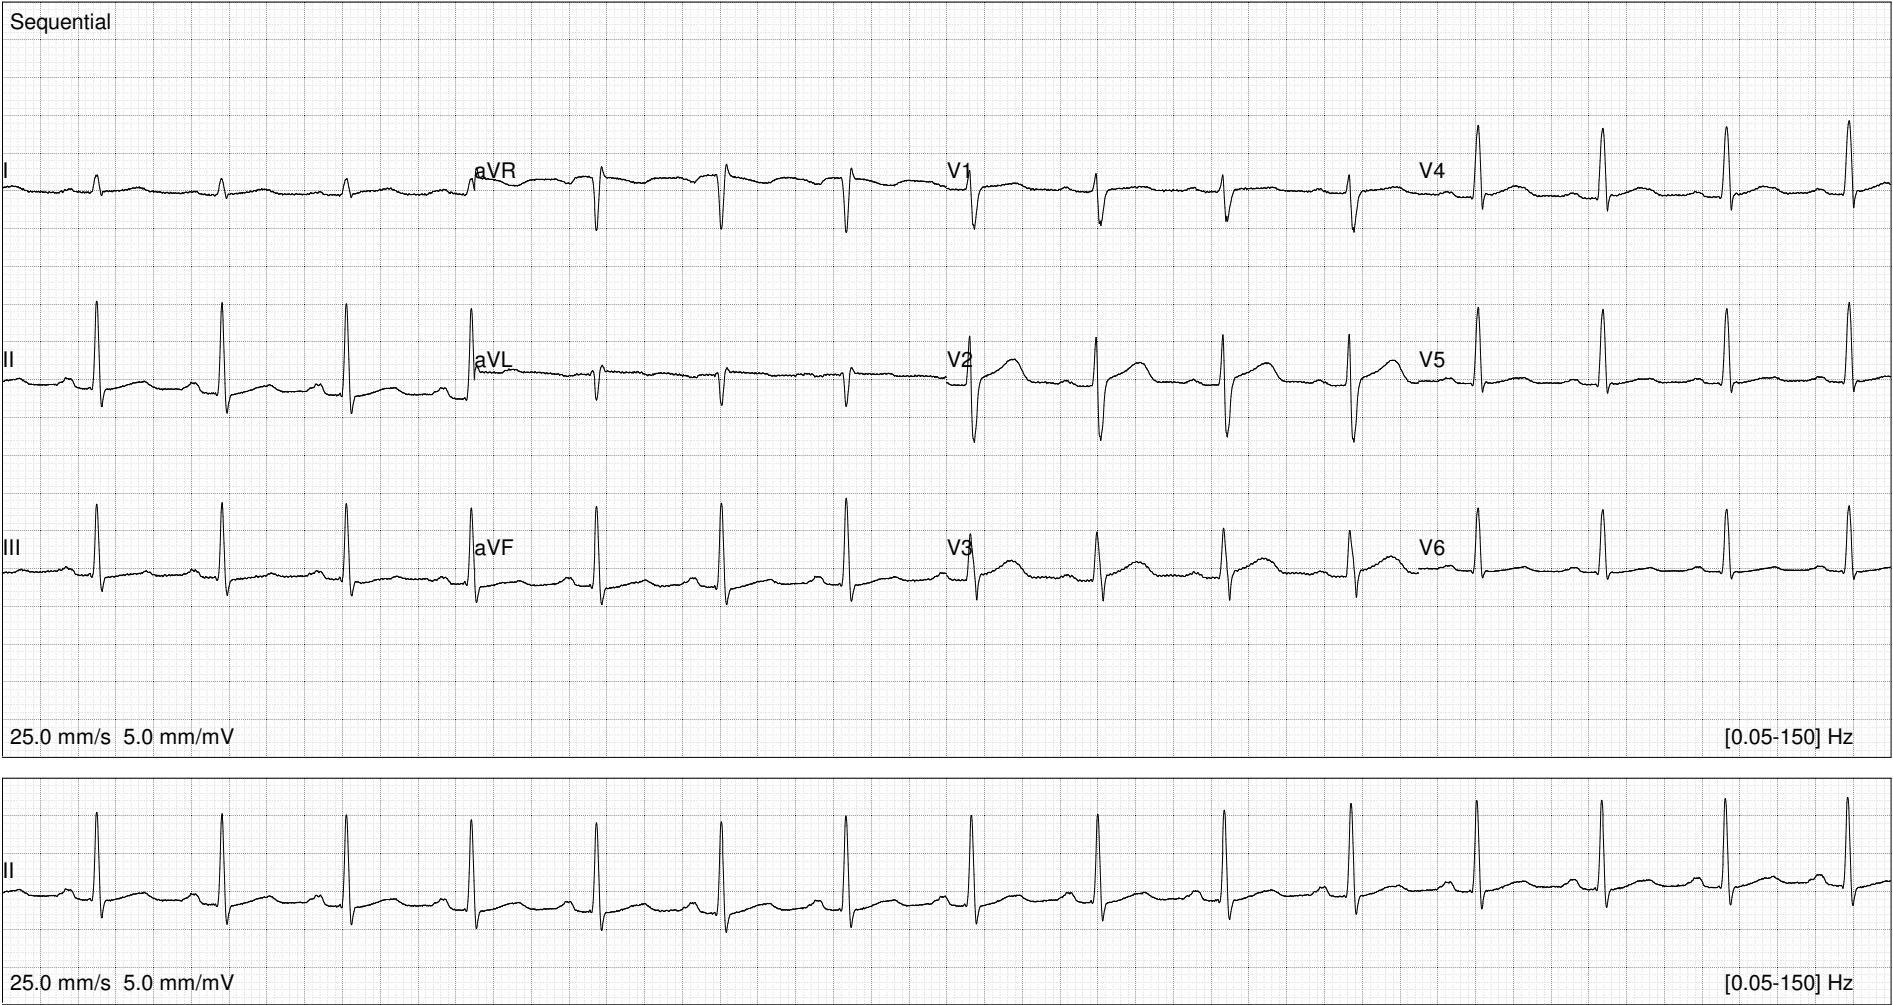

Anton Swart Biokinetic Rehabilitation Practice

Name:

Number:

Gender:

Birthdate:

P / PQ:

QRS:

QT / QTc / QTd:

P/QRS/T axis:

Heartrate:

014 014 014

014

Male

13/06/1972 45 years

112 ms / 173 ms

87 ms

359 ms / 415 ms / -

76° / 78° / 50°

92 bpm

Recorded:

Recorded by:

Referring physician:

Location:

Ordering physician:

Attending physician:

Comment:



03/05/2018 17:07:49

Mr. Anton Swart

Anton Swart Biokinetic Rehabilitation Practice

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW



Beats		RR	
Total:	458	Minimum	590 ms
Normal:	458	Maximum	720 ms
Other:	0	Mean:	653 ms
		SD:	20 ms

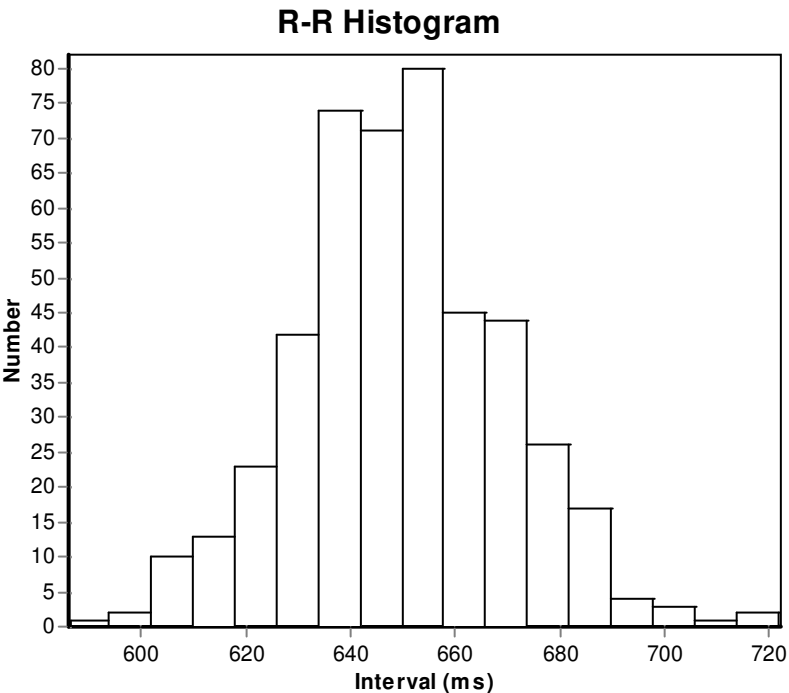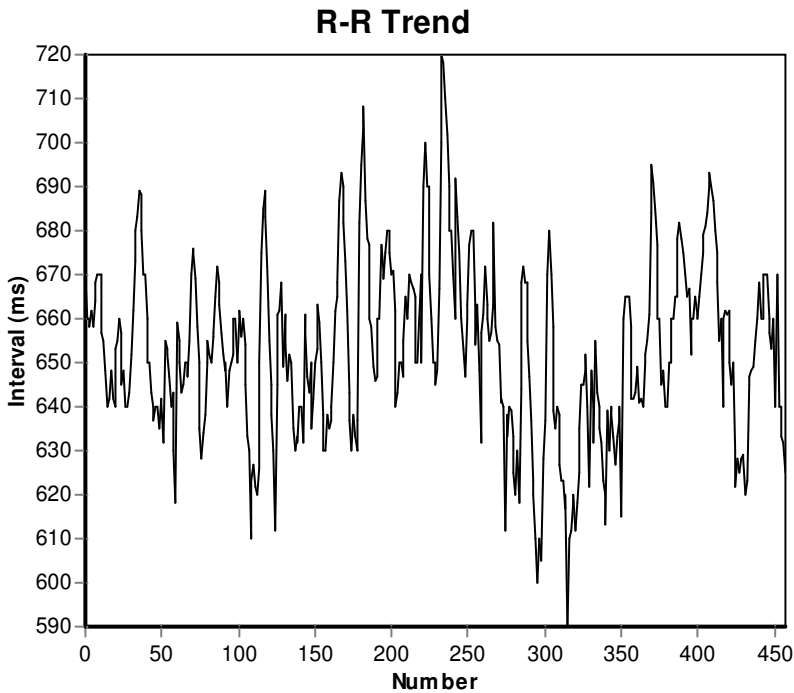

Heart Rate Variability: Time Domain Analysis

Name: 014, 014 014
Number: 014
Gender: Male


Birthdate: 13/06/1972
Recorded: 03/05/2018 17:07:49

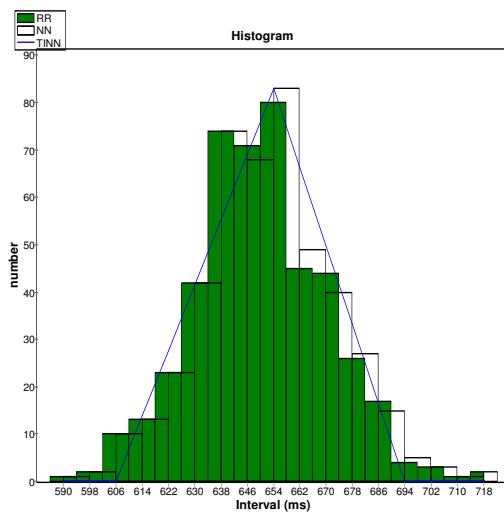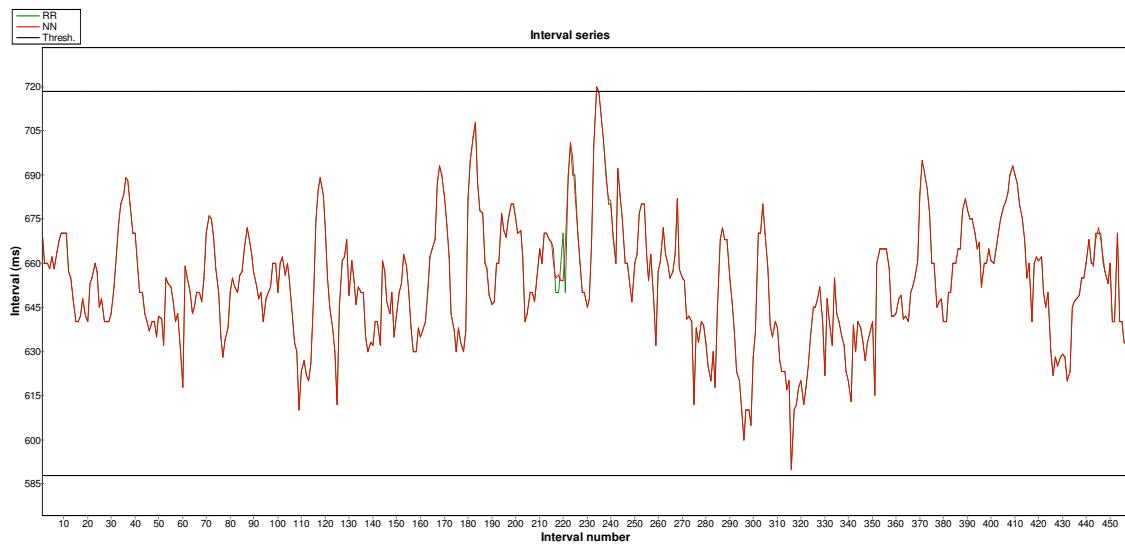

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	20	20
Triangular Interpolation (ms)	88	96
Triangular Index	5.52	5.72

Interval statistics	NN	RR
Number	458	458
Minimum (ms)	590	590
Maximum (ms)	720	720
Range (ms)	130	130
Avg (ms)	653	653
SD (ms)	20	20
AvgDev (ms)	16	16
p5 (ms)	620	620
p50 (ms)	653	652
p95 (ms)	688	689
Skewness	0.15	0.15
Kurtosis	3.24	3.22


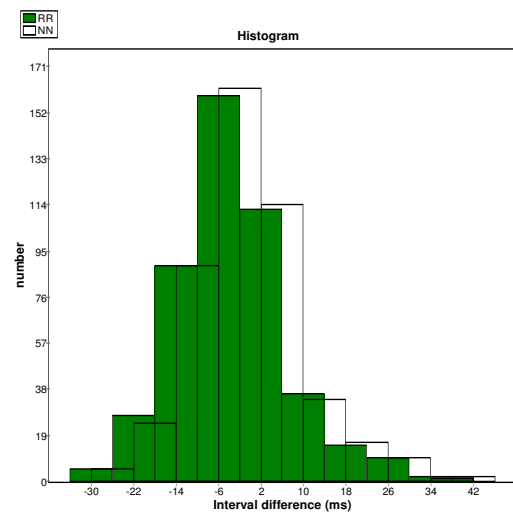


HRV parameters	NN	RR
SDSD (ms)	11	11
RMSSD (ms)	11	11
NN50	0	0
NN50(1)	0	0
NN50(2)	0	0
pNN50	0.00	0.00
pNN50(1)	0.00	0.00
pNN50(2)	0.00	0.00
Logarithmic Index	0.96	0.92
SD(Logarithmic Index)	0.07	0.09

Interval statistics	NN	RR
Number	457	457
Minimum (ms)	-30	-30
Maximum (ms)	45	45
Range (ms)	75	75
Avg (ms)	-0	-0
SD (ms)	11	11
AvgDev (ms)	8	8
p5 (ms)	-15	-16
p50 (ms)	0	0
p95 (ms)	23	23
Skewness	0.82	0.85
Kurtosis	5.28	5.35

Heart Rate Variability: Frequency Domain Analysis

Name: 014, 014 014 Birthdate: 13/06/1972
 Number: 014 Recorded: 03/05/2018 17:07:49
 Gender: Male

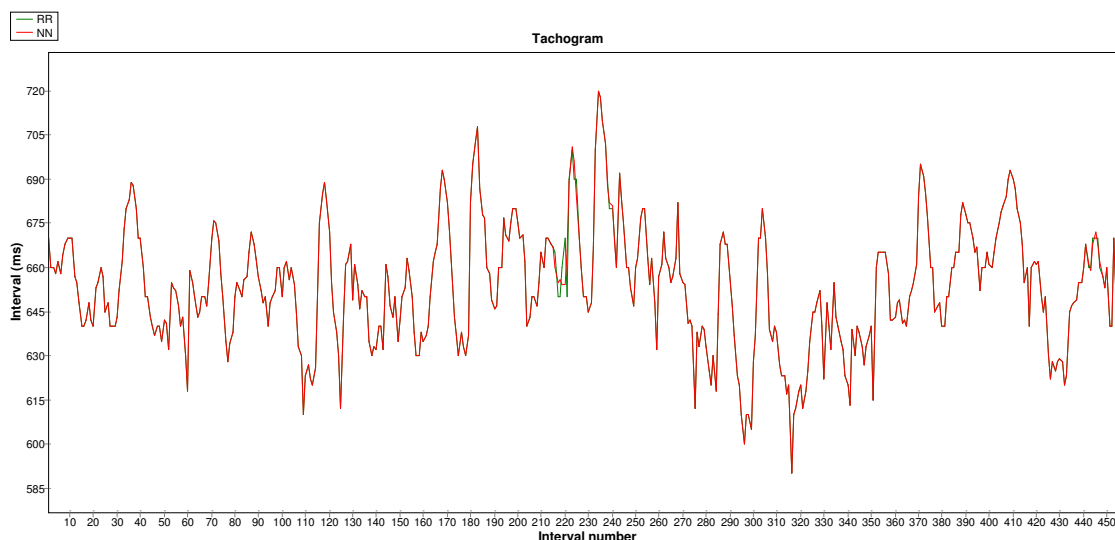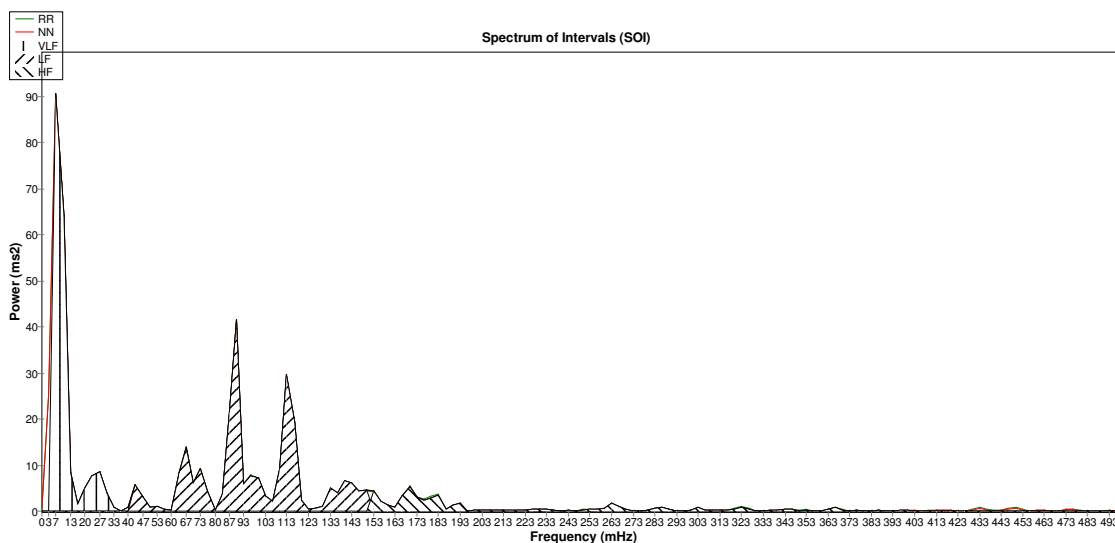

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	484	481	Spectrum of Intervals (SOI)	
VLF (ms2)	192	192	Frequency resolution (mHz)	3
LF (ms2)	240	239	VLF lower boundary (mHz)	3
HF (ms2)	52	51	VLF upper boundary (mHz)	40
LF/HF	4.66	4.69	LF upper boundary (mHz)	150
LF normalized	82.33	82.42	HF upper boundary (mHz)	400
HF normalized	17.67	17.58	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	90	90	Fourier transform	DFT
HF peak (mHz)	170	170	Sample frequency (Hz)	1.53
			Interval correction	Annotation
			Interval threshold (%)	10