


Anton Swart Biokinetic Rehabilitation Practice

Name: 016 016
Number: 016
Gender: Female
Birthdate: 26/11/1970 47 years

P / PQ: 115 ms / 145 ms
QRS: 80 ms
QT / QTc / QTd: 392 ms / 425 ms / -
P/QRS/T axis: 70° / 88° / 75°
Heartrate: 79 bpm

Recorded: 04/05/2018 13:51:01
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

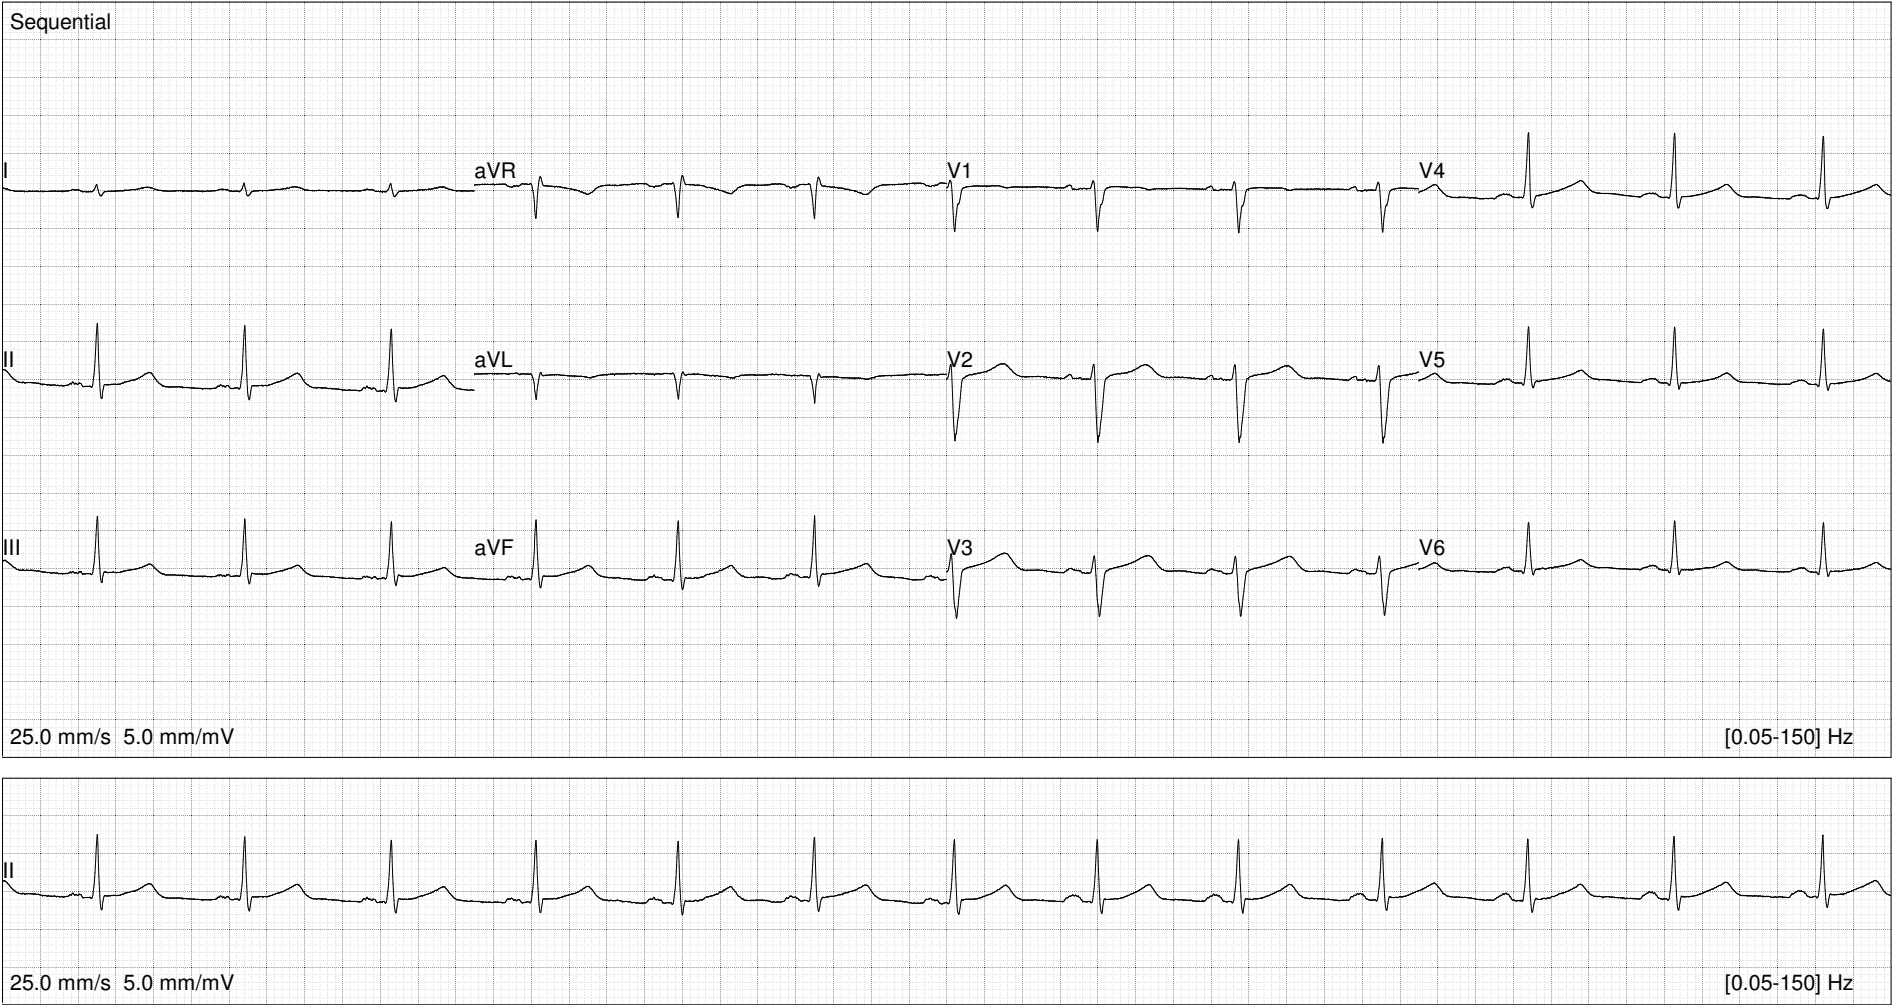

Anton Swart Biokinetic Rehabilitation Practice



Name: 016 016
Number: 016
Gender: Female
Birthdate: 26/11/1970 47 years

P / PQ: 115 ms / 145 ms
QRS: 80 ms
QT / QTc / QTd: 392 ms / 425 ms / -
P/QRS/T axis: 70° / 88° / 75°
Heartrate: 79 bpm

Recorded: 04/05/2018 13:51:01
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:



UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	395	Minimum	698 ms
Normal:	395	Maximum	804 ms
Other:	0	Mean:	757 ms
		SD:	22 ms

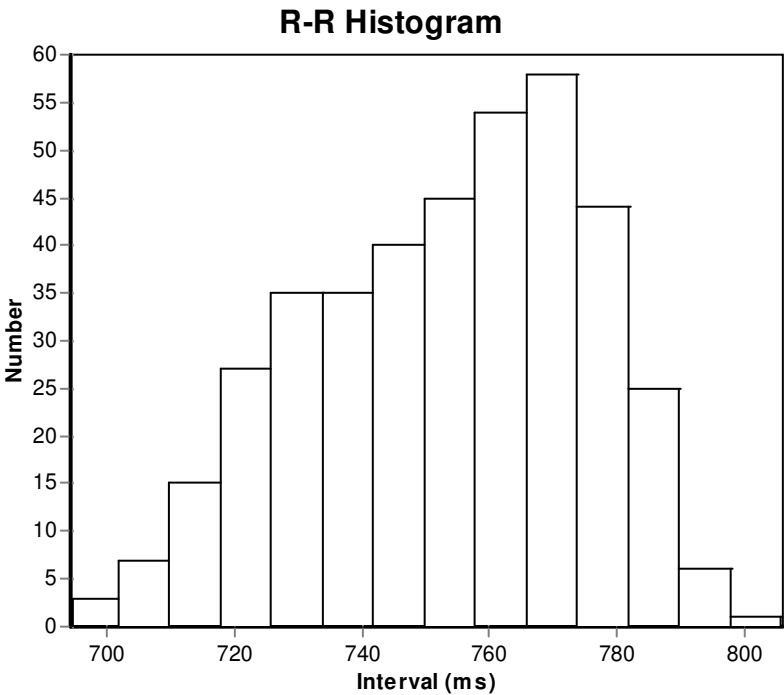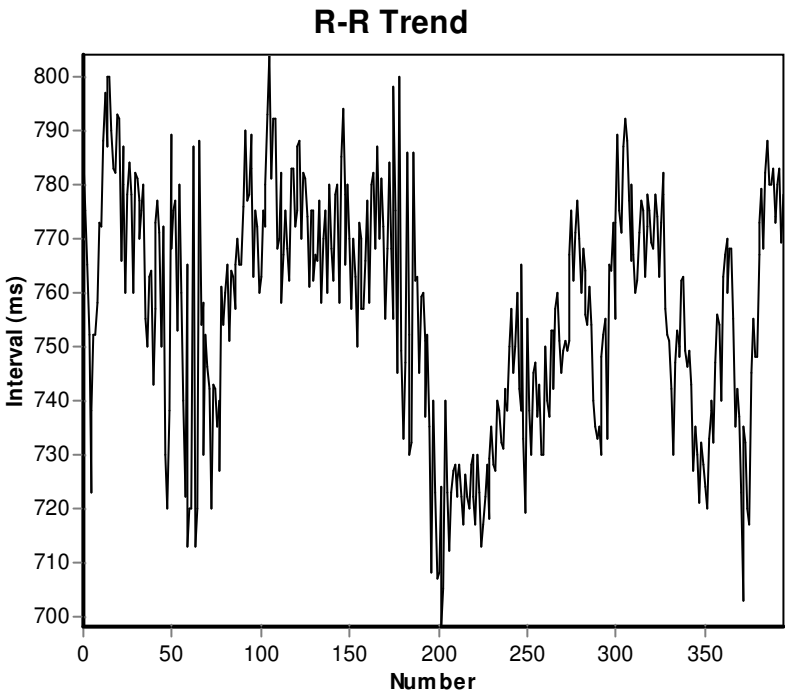

Heart Rate Variability: Time Domain Analysis


Name: 016, 016 Birthdate: 26/11/1970
 Number: 016 Recorded: 04/05/2018 13:51:01
 Gender: Female

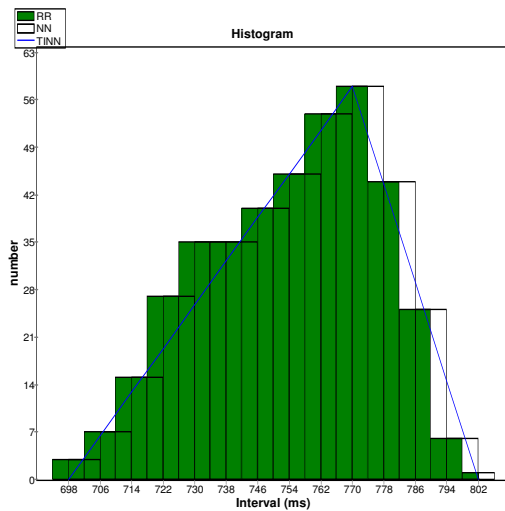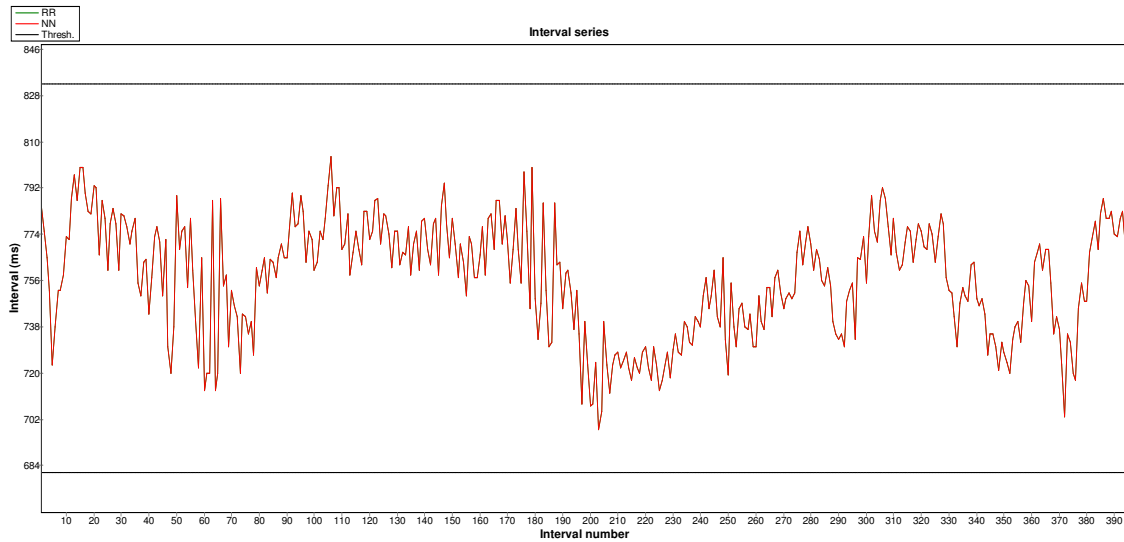

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	22	22
Triangular Interpolation (ms)	104	104
Triangular Index	6.81	6.81

Interval statistics	NN	RR
Number	395	395
Minimum (ms)	698	698
Maximum (ms)	804	804
Range (ms)	106	106
Avg (ms)	757	757
SD (ms)	22	22
AvgDev (ms)	18	18
p5 (ms)	720	720
p50 (ms)	760	760
p95 (ms)	788	788
Skewness	-0.31	-0.31
Kurtosis	2.28	2.28

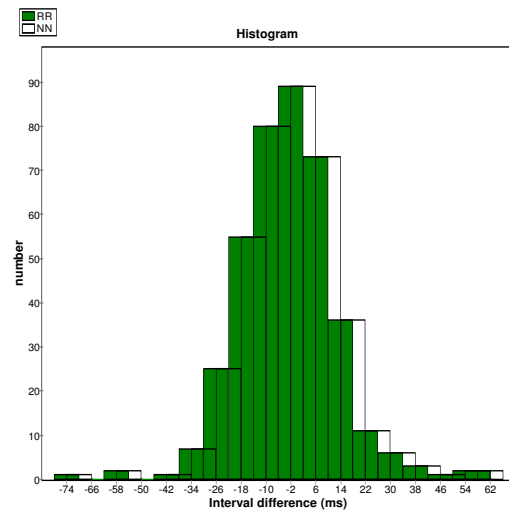



HRV parameters	NN	RR
SDSD (ms)	16	16
RMSSD (ms)	16	16
NN50	8	8
NN50(1)	3	3
NN50(2)	5	5
pNN50	0.02	0.02
pNN50(1)	0.01	0.01
pNN50(2)	0.01	0.01
Logarithmic Index	0.66	0.66
SD(Logarithmic Index)	0.05	0.05

Interval statistics	NN	RR
Number	394	394
Minimum (ms)	-74	-74
Maximum (ms)	68	68
Range (ms)	142	142
Avg (ms)	-0	-0
SD (ms)	16	16
AvgDev (ms)	12	12
p5 (ms)	-23	-23
p50 (ms)	0	0
p95 (ms)	23	23
Skewness	0.31	0.31
Kurtosis	6.12	6.12

Heart Rate Variability: Frequency Domain Analysis

Name: 016, 016
Number: 016
Gender: Female

Birthdate: 26/11/1970
Recorded: 04/05/2018 13:51:01

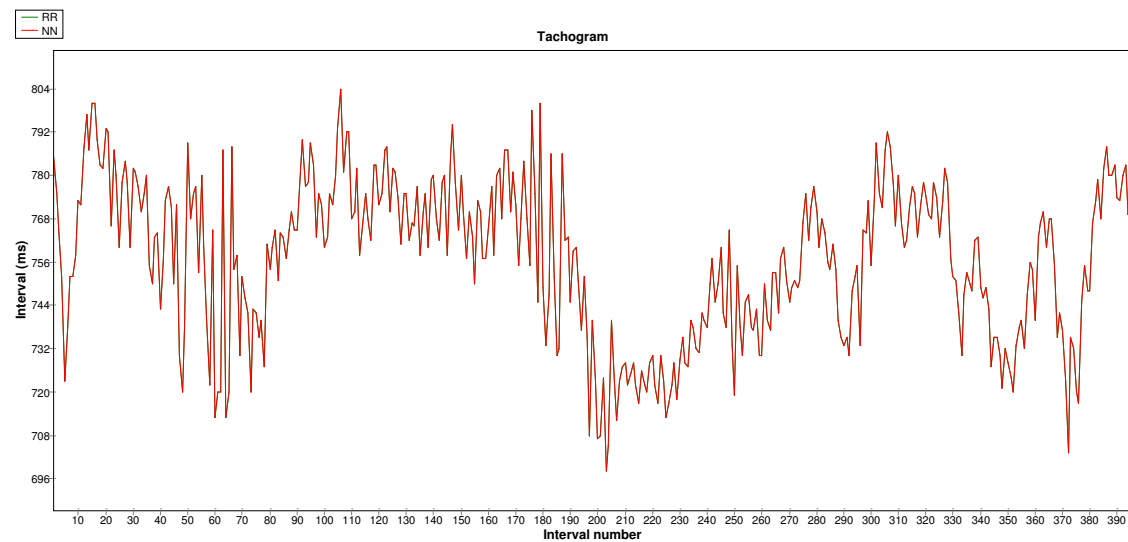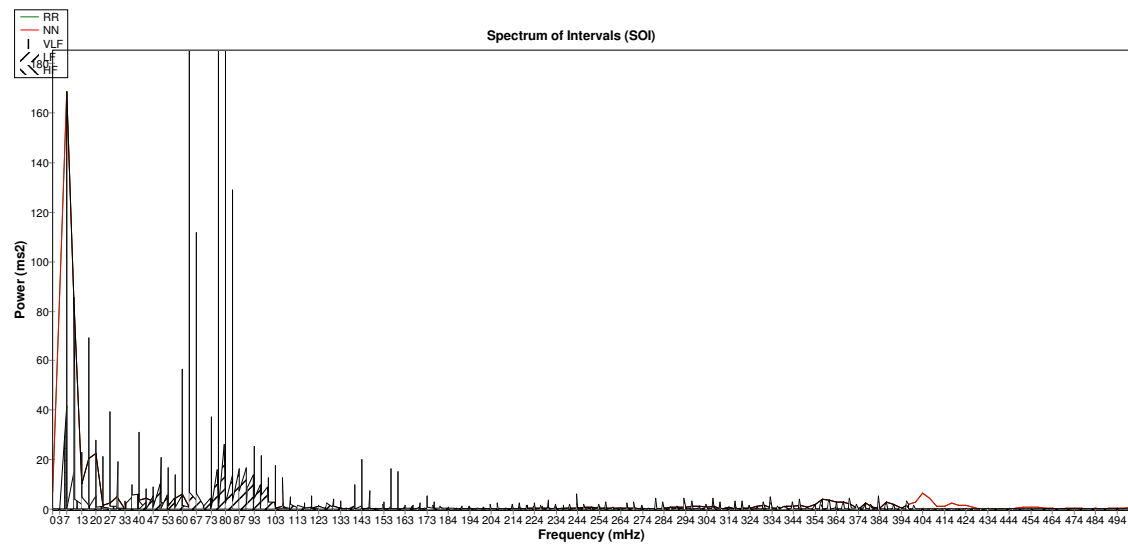

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	426	426	Spectrum of Intervals (SOI)	
VLF (ms2)	323	323	Frequency resolution (mHz)	3
LF (ms2)	47	47	VLF lower boundary (mHz)	3
HF (ms2)	57	57	VLF upper boundary (mHz)	40
LF/HF	0.83	0.83	LF upper boundary (mHz)	150
LF normalized	45.35	45.35	HF upper boundary (mHz)	400
HF normalized	54.65	54.65	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	60	60	Fourier transform	DFT
HF peak (mHz)	357	357	Sample frequency (Hz)	1.32
			Interval correction	Annotation
			Interval threshold (%)	10