


Anton Swart Biokinetic Rehabilitation Practice

Name: 016 016
Number: 016
Gender: Female
Birthdate: 26/11/1970 47 years

P / PQ: 92 ms / 132 ms
QRS: 78 ms
QT / QTc / QTd: 451 ms / 448 ms / -
P/QRS/T axis: 38° / 91° / 78°
Heartrate: 58 bpm

Recorded: 06/05/2018 09:18:36
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

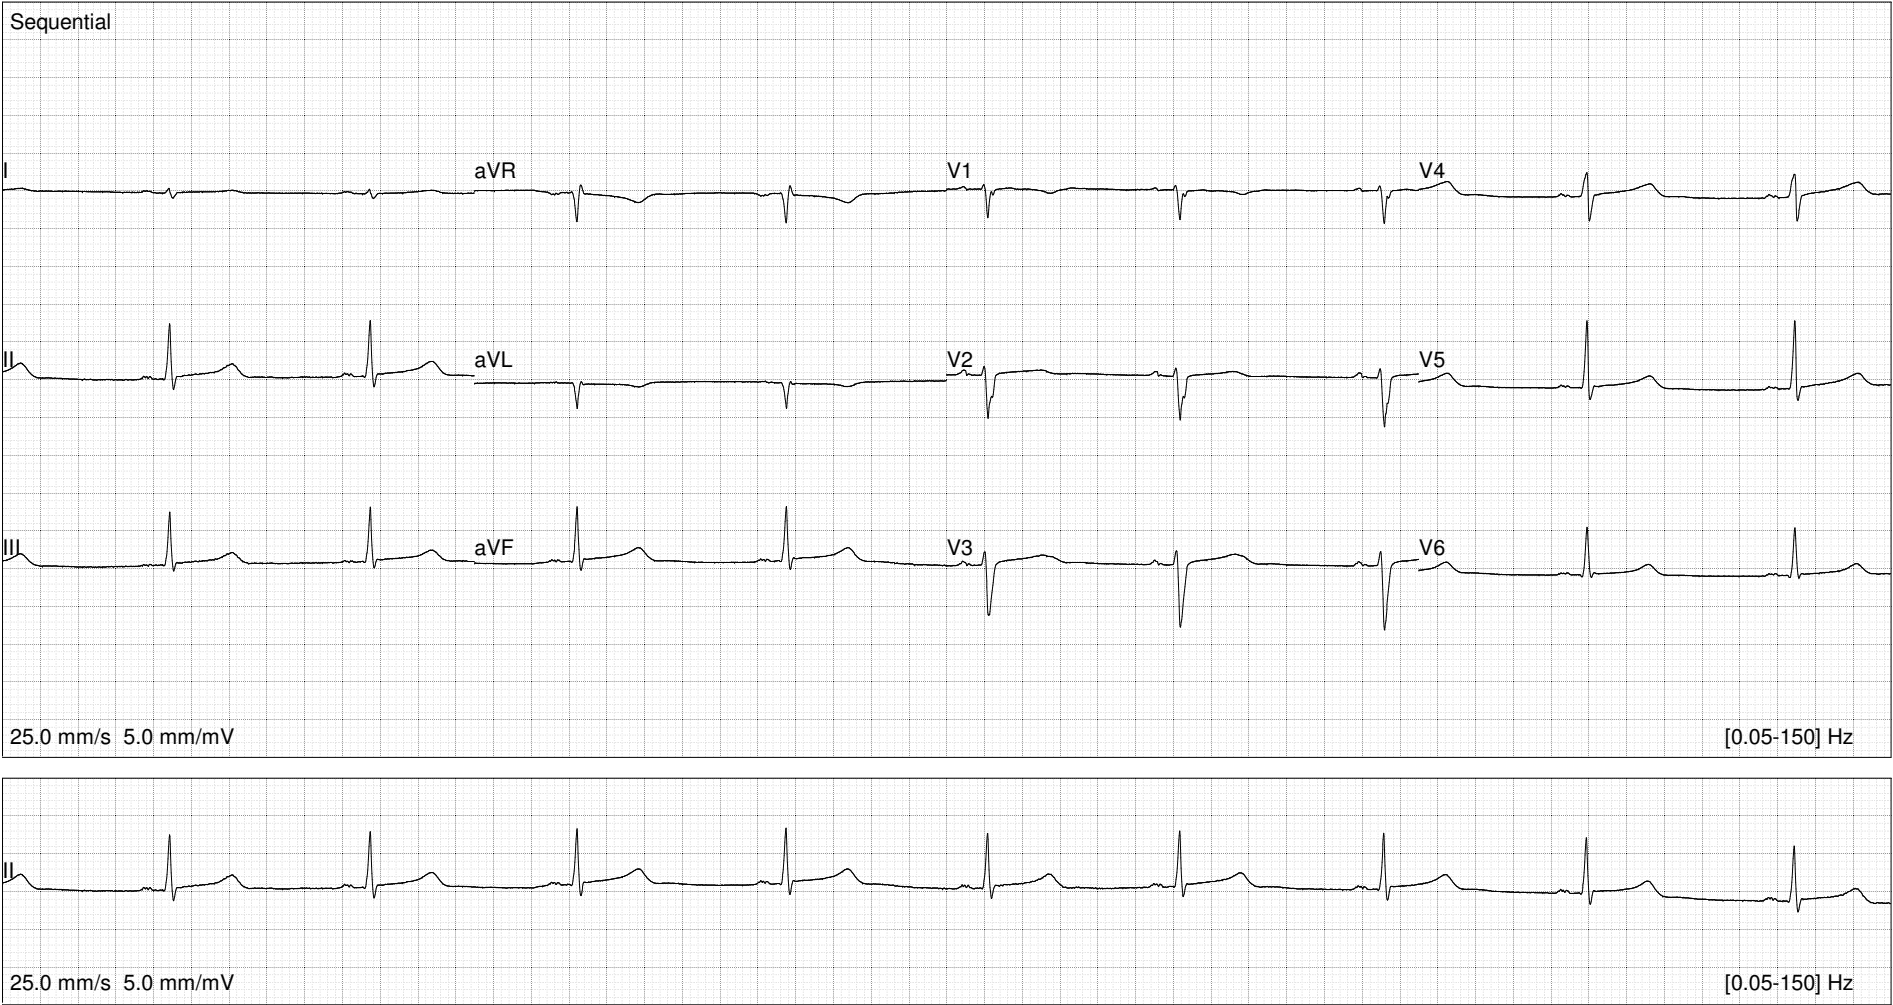

Anton Swart Biokinetic Rehabilitation Practice

Name: 016 016
Number: 016
Gender: Female
Birthdate: 26/11/1970 47 years


P / PQ: 92 ms / 132 ms
QRS: 78 ms
QT / QTc / QTd: 451 ms / 448 ms / -
P/QRS/T axis: 38° / 91° / 78°
Heartrate: 58 bpm

Recorded: 06/05/2018 09:18:36
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:


UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	288	Minimum	910 ms
Normal:	288	Maximum	1188 ms
Other:	0	Mean:	1036 ms
		SD:	49 ms

R-R Trend


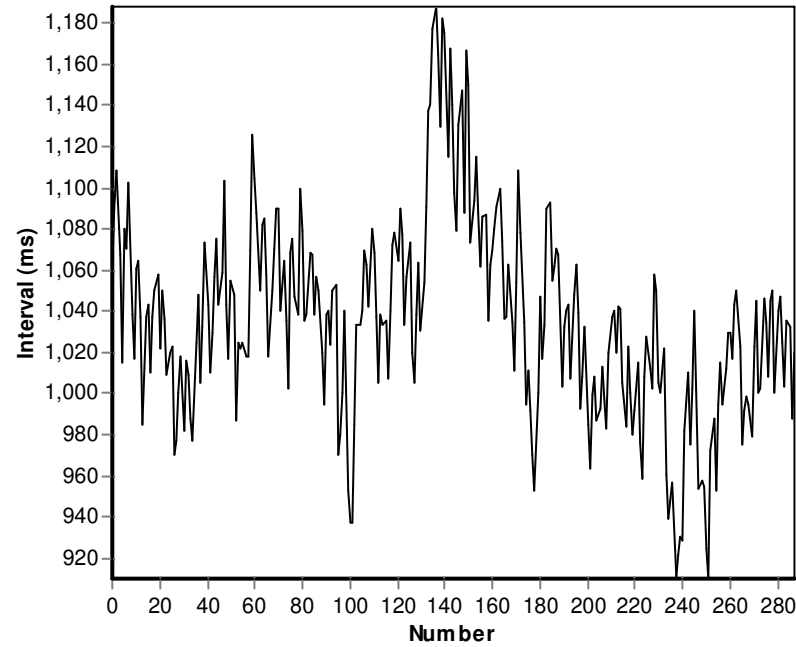


R-R Histogram

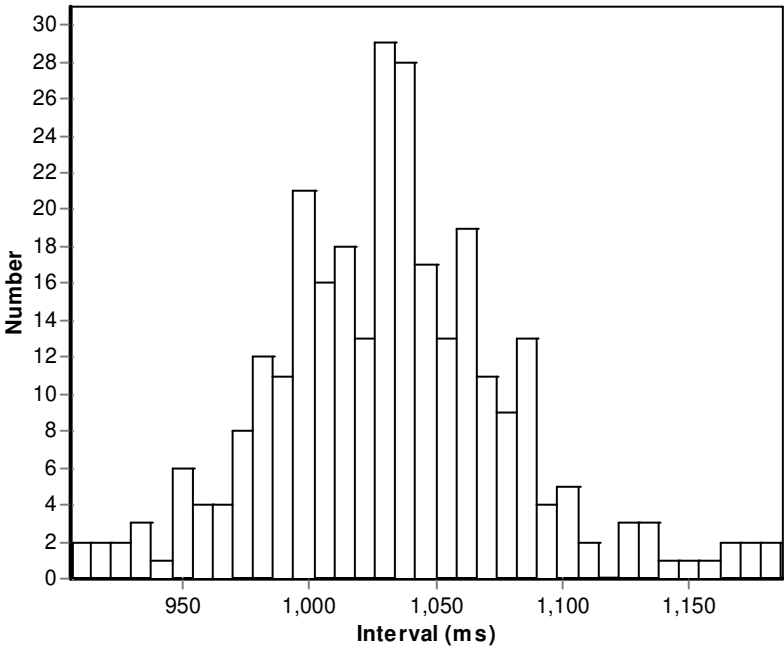

Heart Rate Variability: Time Domain Analysis


Name: 016, 016 Birthdate: 26/11/1970
 Number: 016 Recorded: 06/05/2018 09:18:36
 Gender: Female

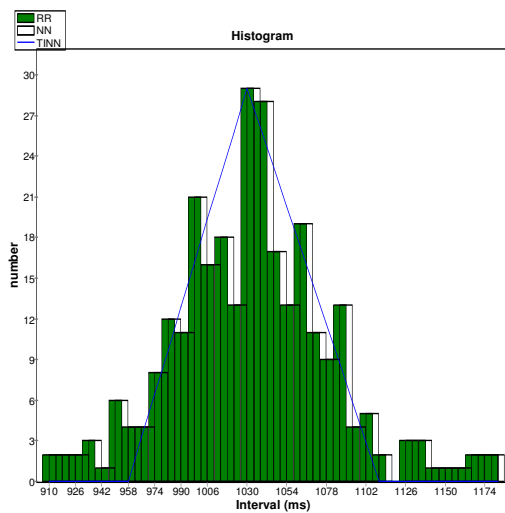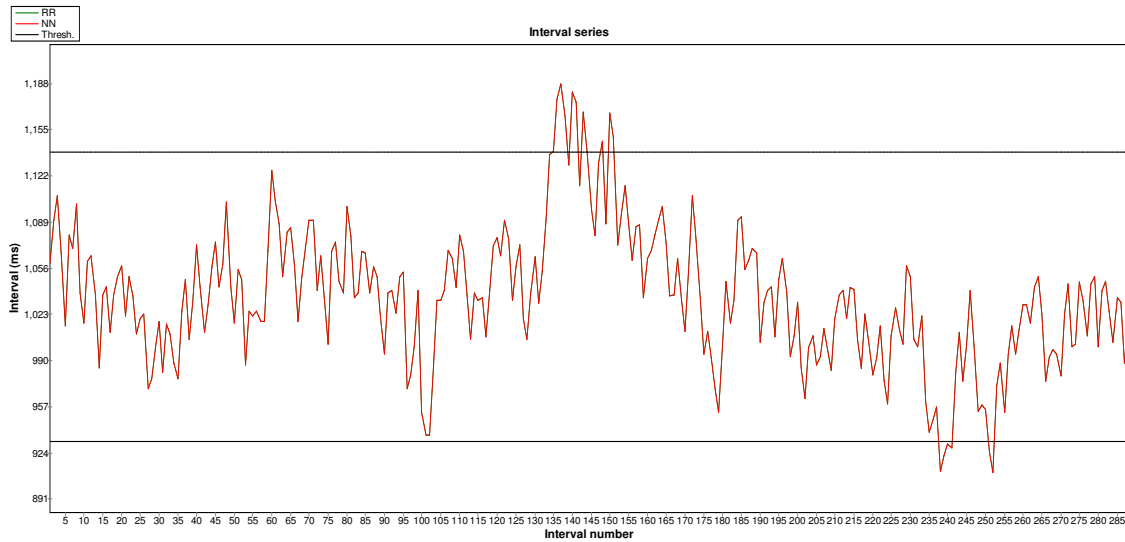

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	49	49
Triangular Interpolation (ms)	152	152
Triangular Index	9.93	9.93

Interval statistics	NN	RR
Number	288	288
Minimum (ms)	910	910
Maximum (ms)	1188	1188
Range (ms)	278	278
Avg (ms)	1036	1036
SD (ms)	49	49
AvgDev (ms)	37	37
p5 (ms)	955	955
p50 (ms)	1036	1036
p95 (ms)	1128	1128
Skewness	0.35	0.35
Kurtosis	3.76	3.76


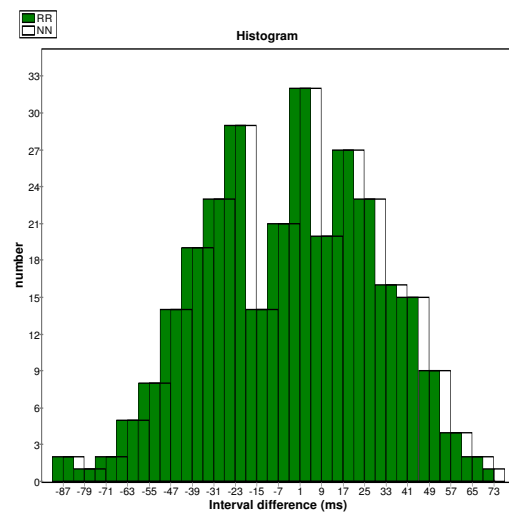


HRV parameters	NN	RR
SDSD (ms)	32	32
RMSSD (ms)	32	32
NN50	30	30
NN50(1)	15	15
NN50(2)	15	15
pNN50	0.10	0.10
pNN50(1)	0.05	0.05
pNN50(2)	0.05	0.05
Logarithmic Index	0.35	0.35
SD(Logarithmic Index)	0.05	0.05

Interval statistics	NN	RR
Number	287	287
Minimum (ms)	-87	-87
Maximum (ms)	79	79
Range (ms)	166	166
Avg (ms)	-0	-0
SD (ms)	32	32
AvgDev (ms)	27	27
p5 (ms)	-52	-52
p50 (ms)	3	3
p95 (ms)	52	52
Skewness	-0.10	-0.10
Kurtosis	2.39	2.39

Heart Rate Variability: Frequency Domain Analysis

Name: 016, 016 Birthdate: 26/11/1970
 Number: 016 Recorded: 06/05/2018 09:18:36
 Gender: Female

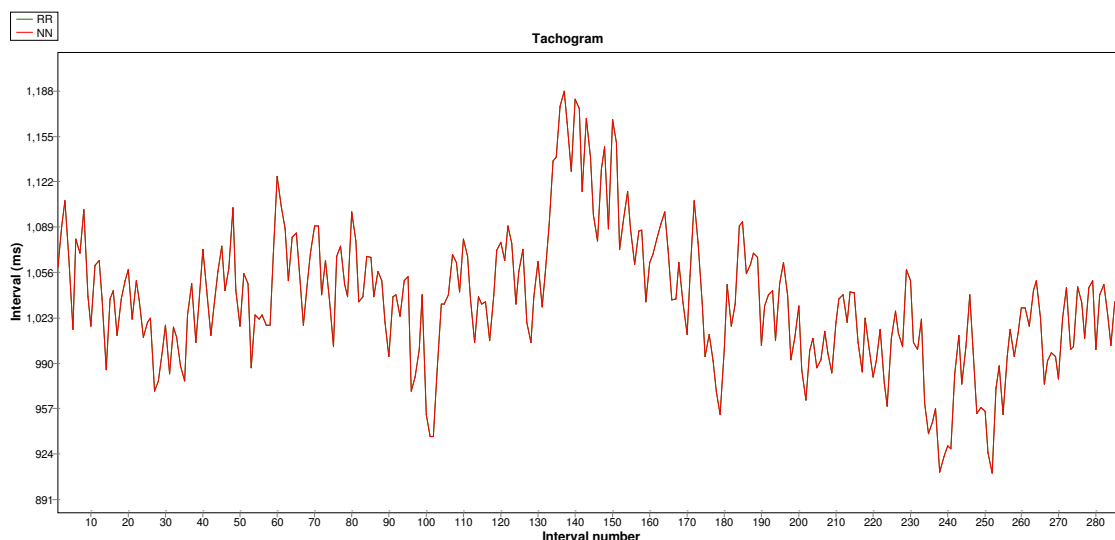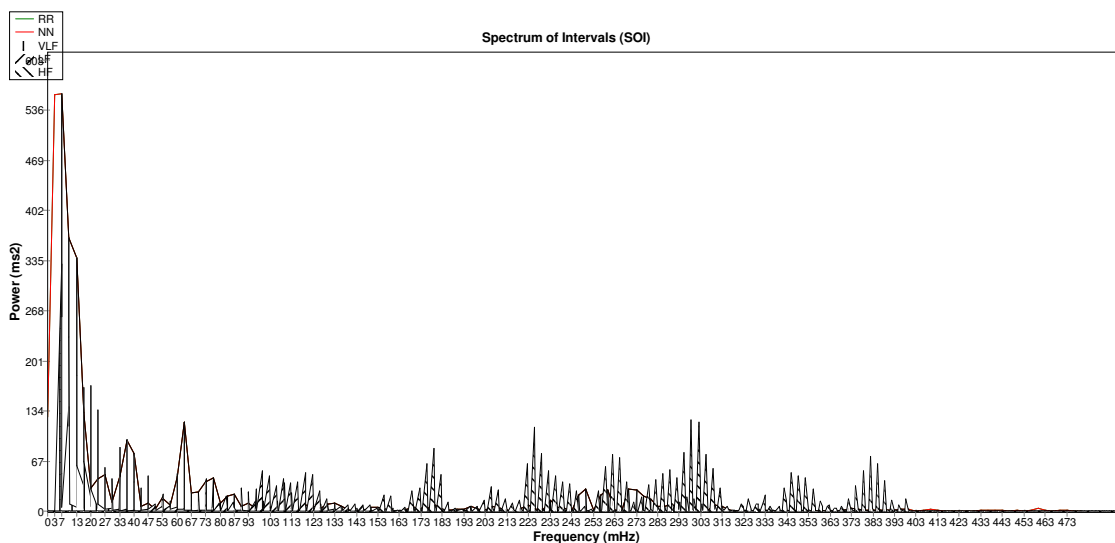

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	2627	2627	Spectrum of Intervals (SOI)	
VLF (ms2)	1751	1751	Frequency resolution (mHz)	3
LF (ms2)	496	496	VLF lower boundary (mHz)	3
HF (ms2)	380	380	VLF upper boundary (mHz)	40
LF/HF	1.30	1.30	LF upper boundary (mHz)	150
LF normalized	56.61	56.61	HF upper boundary (mHz)	400
HF normalized	43.39	43.39	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	63	63	Fourier transform	DFT
HF peak (mHz)	250	250	Sample frequency (Hz)	0.97
			Interval correction	Annotation
			Interval threshold (%)	10