


Anton Swart Biokinetic Rehabilitation Practice

Name: 017 017
Number: 017
Gender: Male
Birthdate: 17/11/1971 46 years

Recorded: 03/05/2018 17:14:49
Recorded by: Mr. Anton Swart
Referring physician:
Ordering physician:
Attending physician:
Location: Anton Swart Biokinetic Rehabilitation Practi
Comment:

UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

P / PQ: 122 ms / 182 ms
QRS: 111 ms
QT / QTc / QTd: 375 ms / 394 ms / -
P/QRS/T axis: 74° / 87° / 79°
Heartrate: 71 bpm

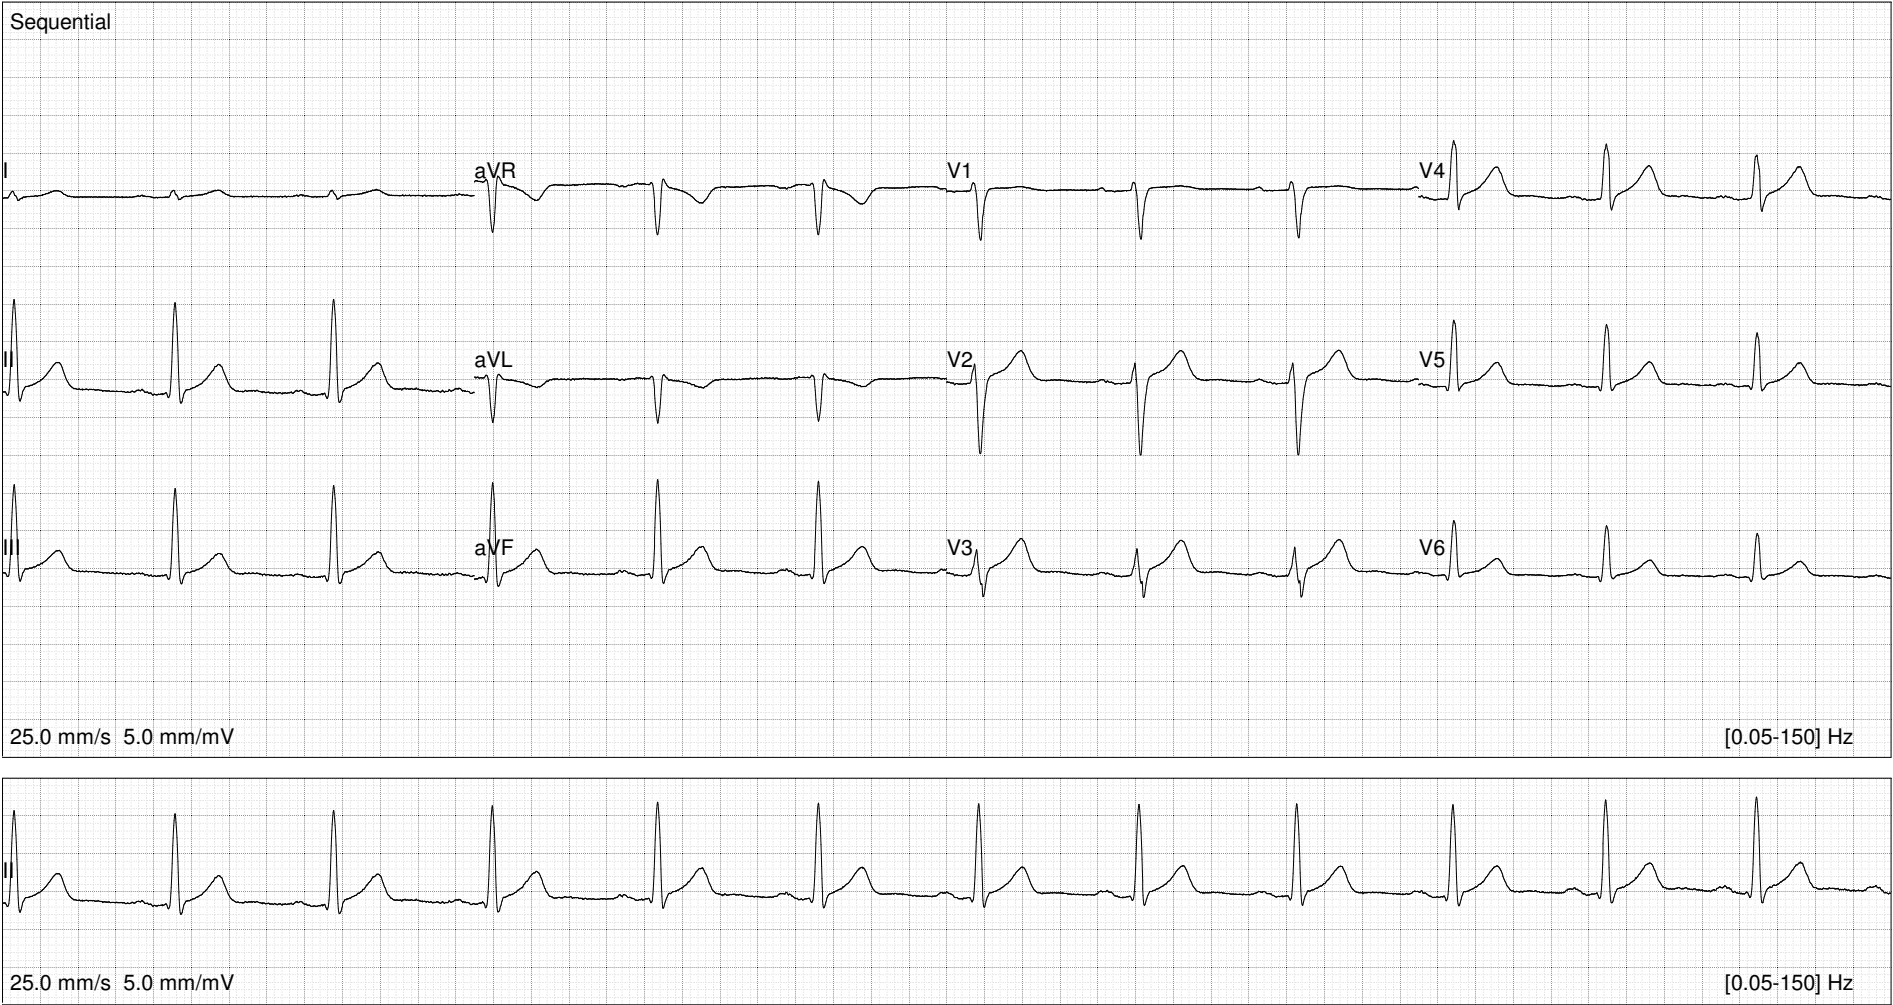

Anton Swart Biokinetic Rehabilitation Practice



Name: 017 017
Number: 017
Gender: Male
Birthdate: 17/11/1971 46 years

P / PQ: 122 ms / 182 ms
QRS: 111 ms
QT / QTc / QTd: 375 ms / 394 ms / -
P/QRS/T axis: 74° / 87° / 79°
Heartrate: 71 bpm

Recorded: 03/05/2018 17:14:49
Recorded by: Mr. Anton Swart
Referring physician:
Location: Anton Swart Biokinetic Rehabilitation Practice
Ordering physician:
Attending physician:
Comment:



UNCONFIRMED INTERPRETATION - MD SHOULD REVIEW

Beats		RR	
Total:	360	Minimum	733 ms
Normal:	360	Maximum	951 ms
Other:	0	Mean:	832 ms
		SD:	35 ms

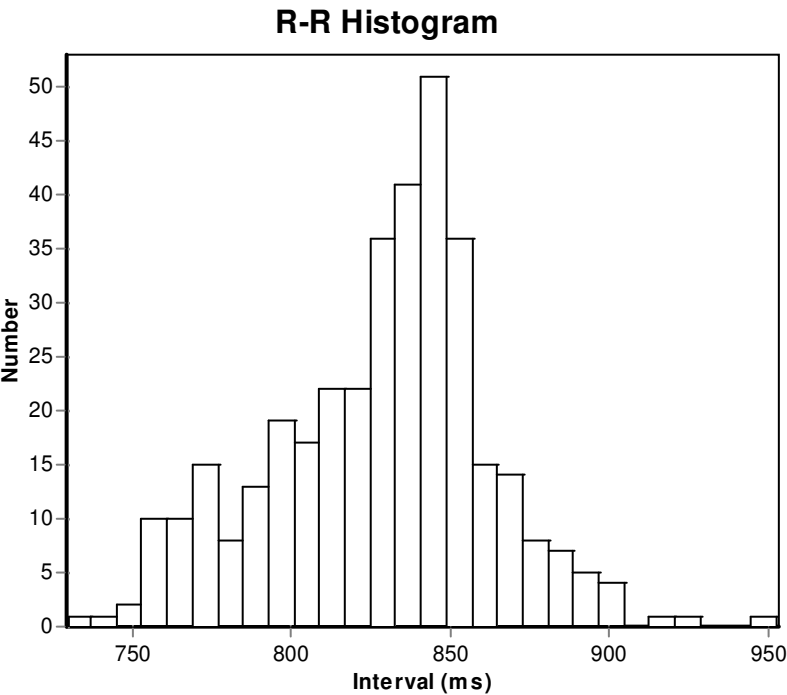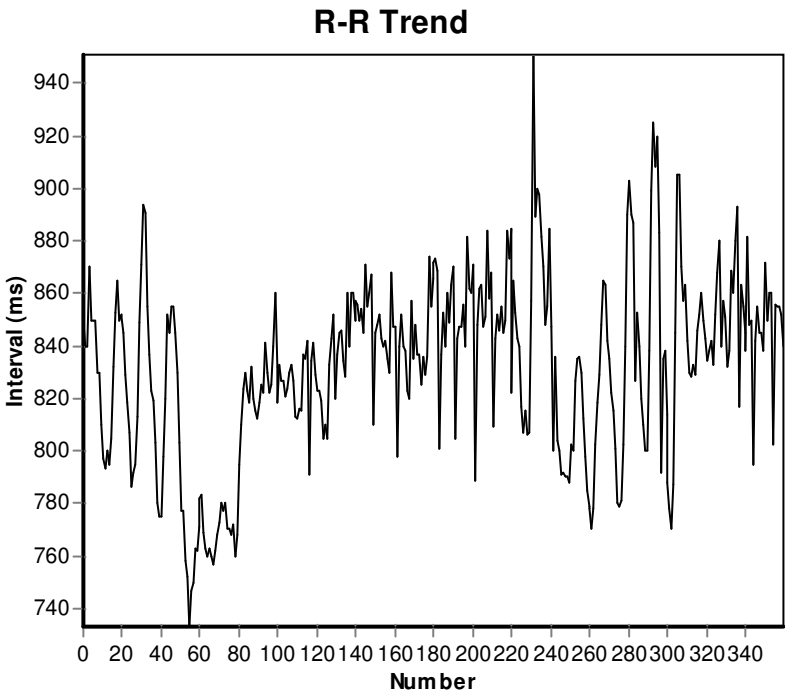

Heart Rate Variability: Time Domain Analysis


Name: 017, 017 Birthdate: 17/11/1971
 Number: 017 Recorded: 03/05/2018 17:14:49
 Gender: Male

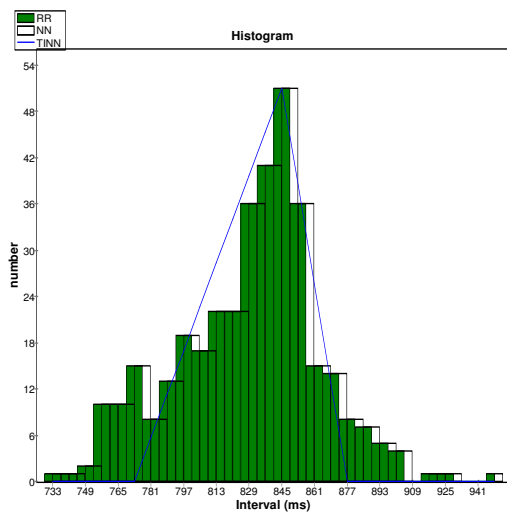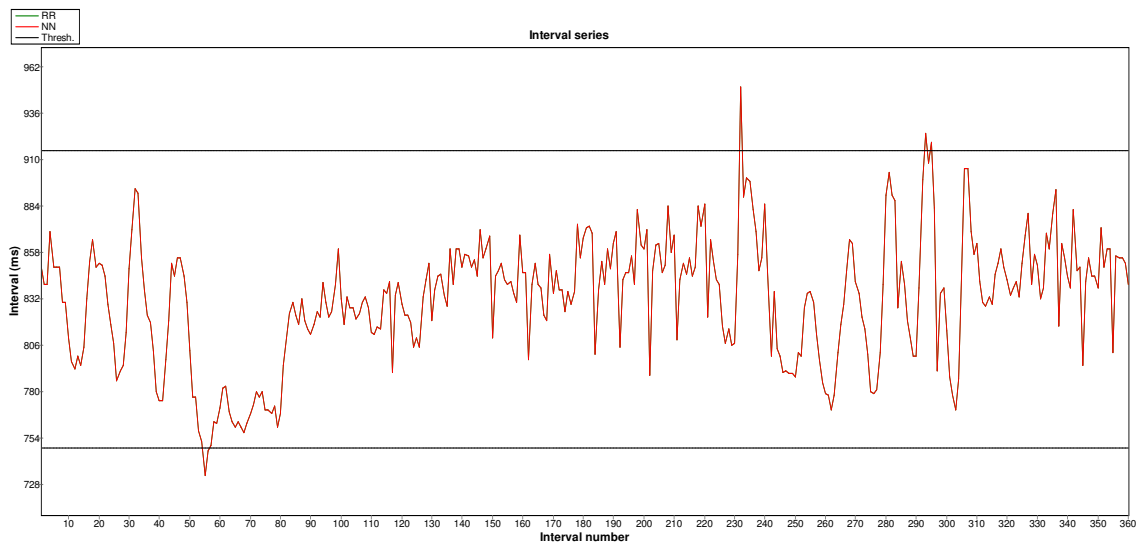

Binsize (ms) = 8

HRV parameters	NN	RR
SDNN (ms)	35	35
Triangular Interpolation (ms)	104	104
Triangular Index	7.06	7.06

Interval statistics	NN	RR
Number	360	360
Minimum (ms)	733	733
Maximum (ms)	951	951
Range (ms)	218	218
Avg (ms)	832	832
SD (ms)	35	35
AvgDev (ms)	27	27
p5 (ms)	770	770
p50 (ms)	837	837
p95 (ms)	885	885
Skewness	-0.20	-0.20
Kurtosis	3.13	3.13

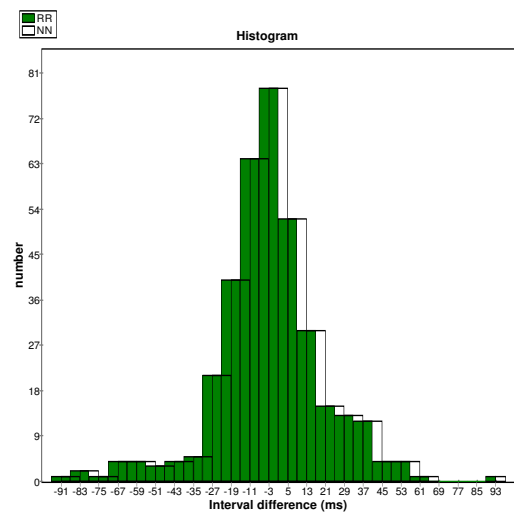



HRV parameters	NN	RR
SDSD (ms)	23	23
RMSSD (ms)	23	23
NN50	19	19
NN50(1)	13	13
NN50(2)	6	6
pNN50	0.05	0.05
pNN50(1)	0.04	0.04
pNN50(2)	0.02	0.02
Logarithmic Index	0.45	0.45
SD(Logarithmic Index)	0.04	0.04

Interval statistics	NN	RR
Number	359	359
Minimum (ms)	-91	-91
Maximum (ms)	94	94
Range (ms)	185	185
Avg (ms)	-0	-0
SD (ms)	23	23
AvgDev (ms)	16	16
p5 (ms)	-37	-37
p50 (ms)	0	0
p95 (ms)	38	38
Skewness	-0.23	-0.23
Kurtosis	5.50	5.50

Heart Rate Variability: Frequency Domain Analysis

Name: 017, 017
Number: 017
Gender: Male

Birthdate: 17/11/1971
Recorded: 03/05/2018 17:14:49

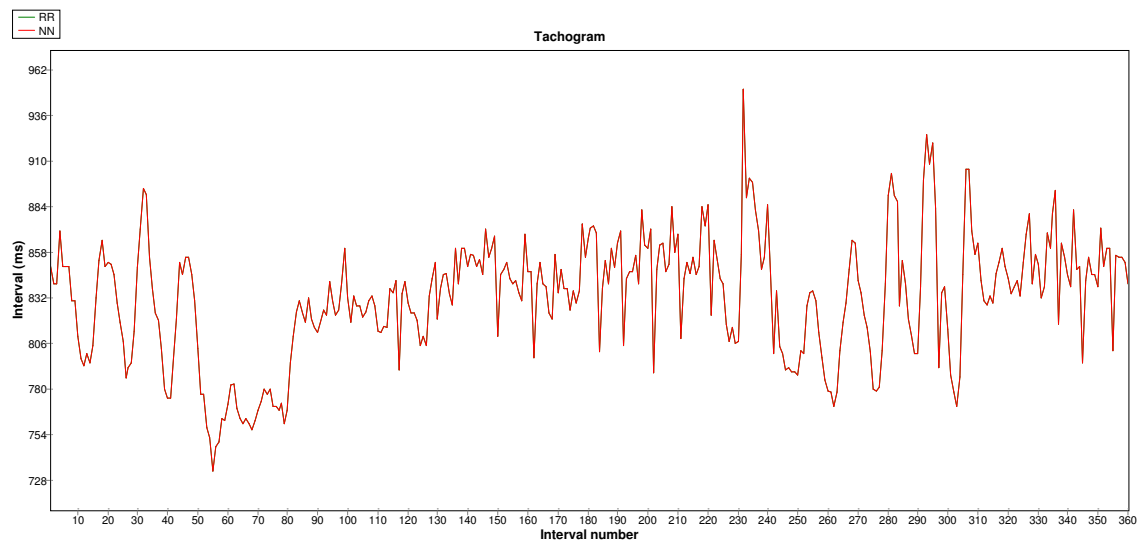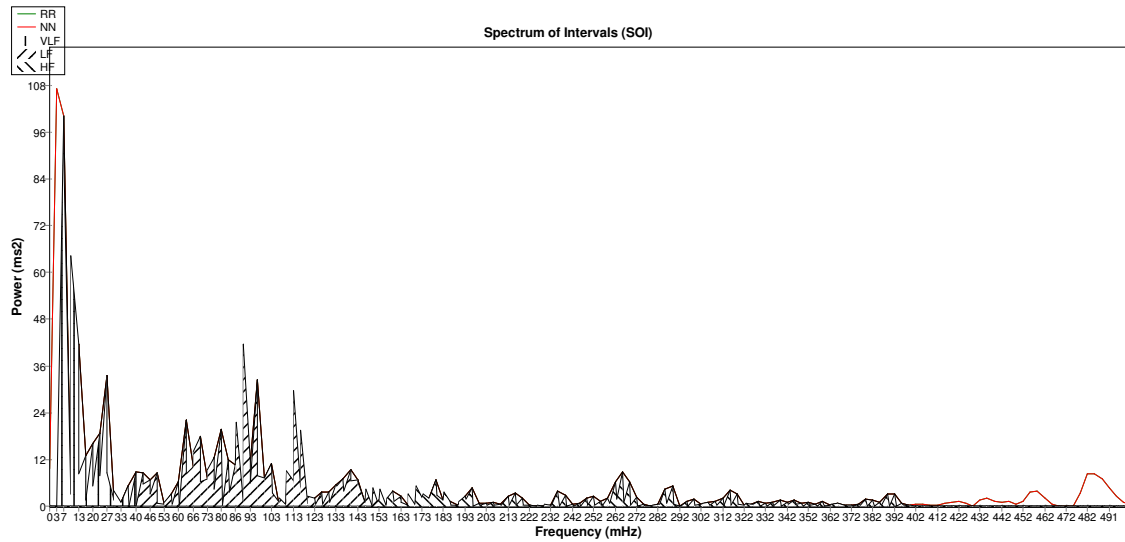

HRV parameters	NN	RR	HRV spectral settings	
TP (ms2)	638	638	Spectrum of Intervals (SOI)	
VLF (ms2)	243	243	Frequency resolution (mHz)	3
LF (ms2)	263	263	VLF lower boundary (mHz)	3
HF (ms2)	133	133	VLF upper boundary (mHz)	40
LF/HF	1.98	1.98	LF upper boundary (mHz)	150
LF normalized	66.45	66.45	HF upper boundary (mHz)	400
HF normalized	33.55	33.55	Smoothing factor	1
VLF peak (mHz)	7	7	Tapering	Hann
LF peak (mHz)	96	96	Fourier transform	DFT
HF peak (mHz)	266	266	Sample frequency (Hz)	1.20
			Interval correction	Annotation
			Interval threshold (%)	10