
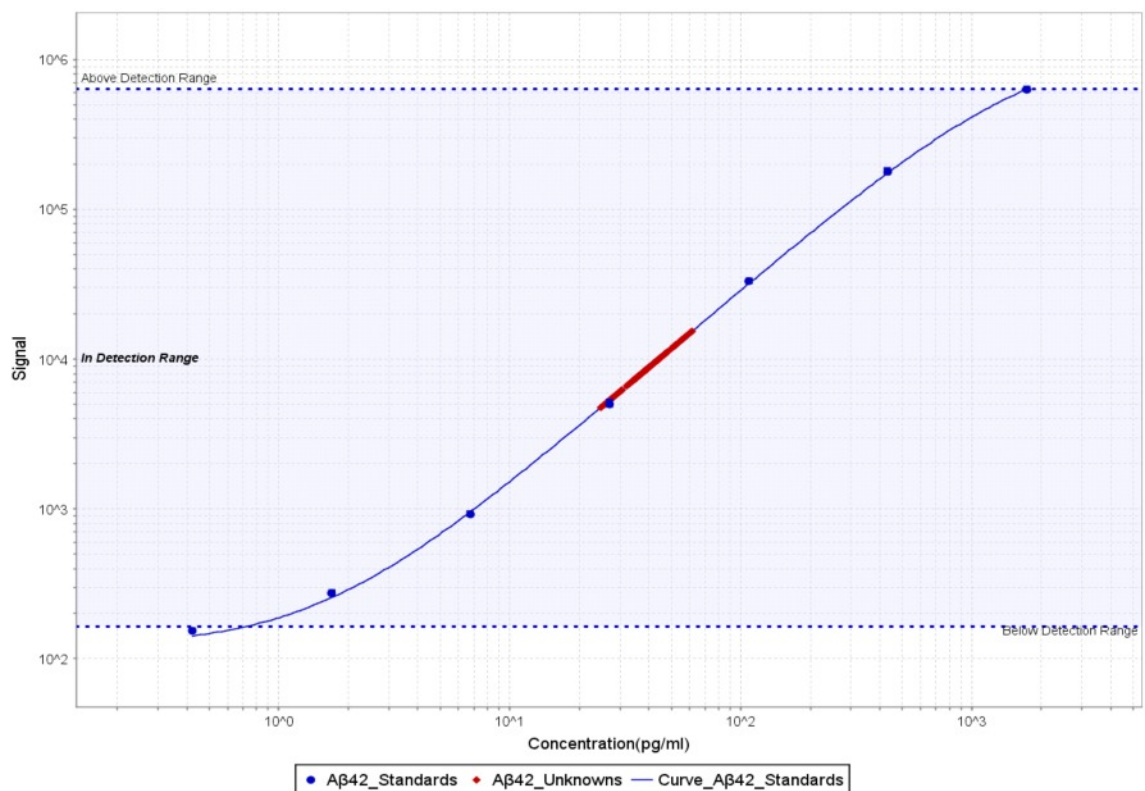


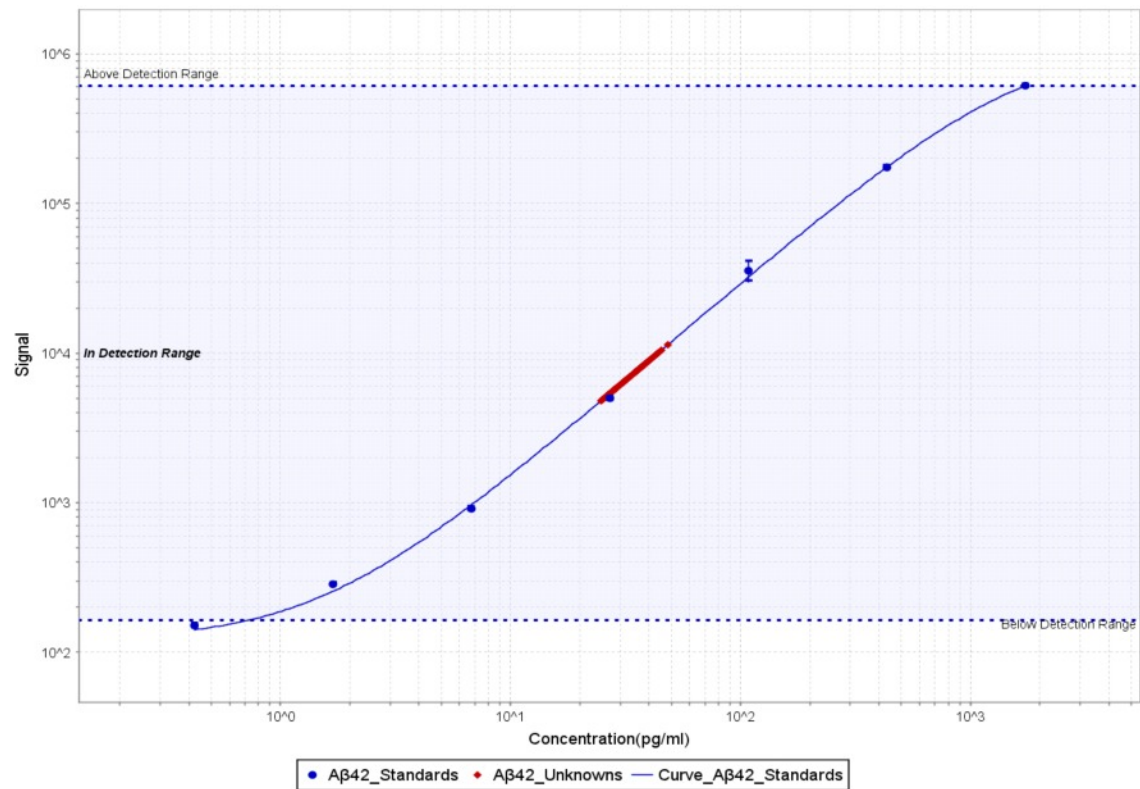

Additional Figure 3: Aβ42 standard curves of the two MSD-assay plates applied to the analysis of the clinical sample. The graphs show the signals of the four-fold dilution series of the Aβ42 calibrator peptide and the standard curves in blue. The signals obtained with the diluted IP eluates are shown in red. The bottom and top of the detection range are defined as the LLOD of the assay plate and the highest calibrator concentration, respectively.