


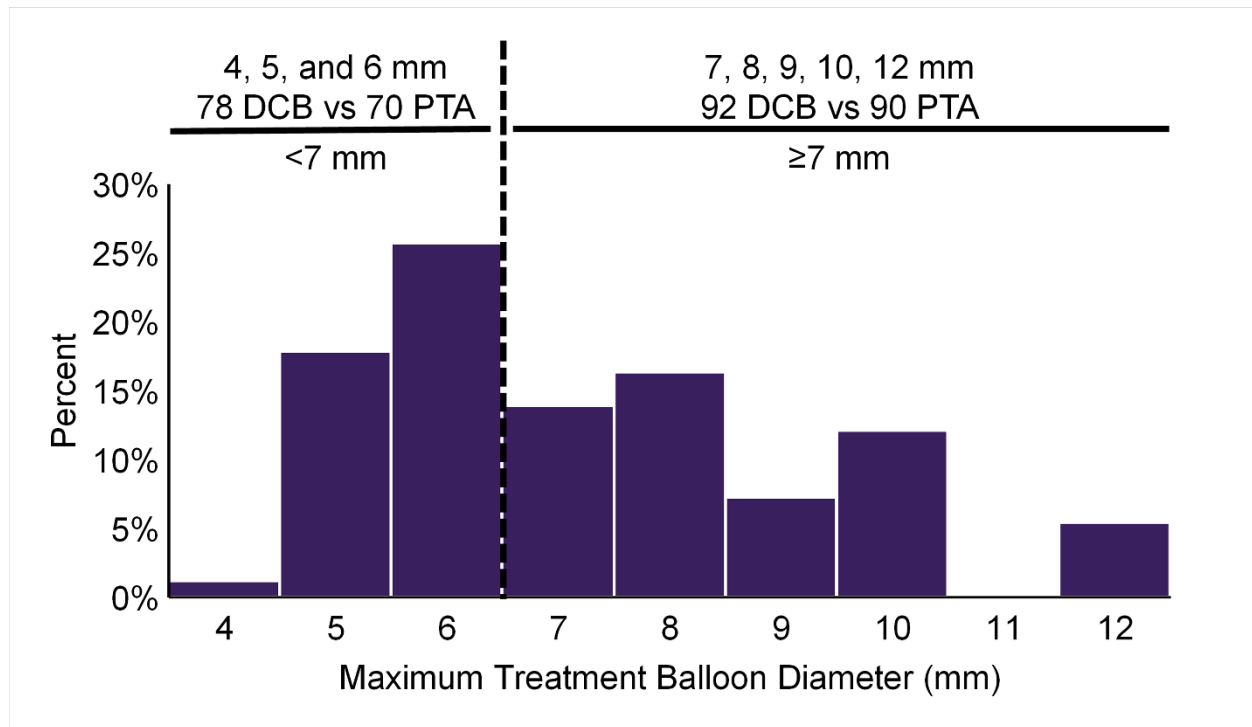

Supplemental Figure 1 – Distribution of site-reported balloon diameter

DCB, drug-coated balloon; PTA, percutaneous transluminal angioplasty